

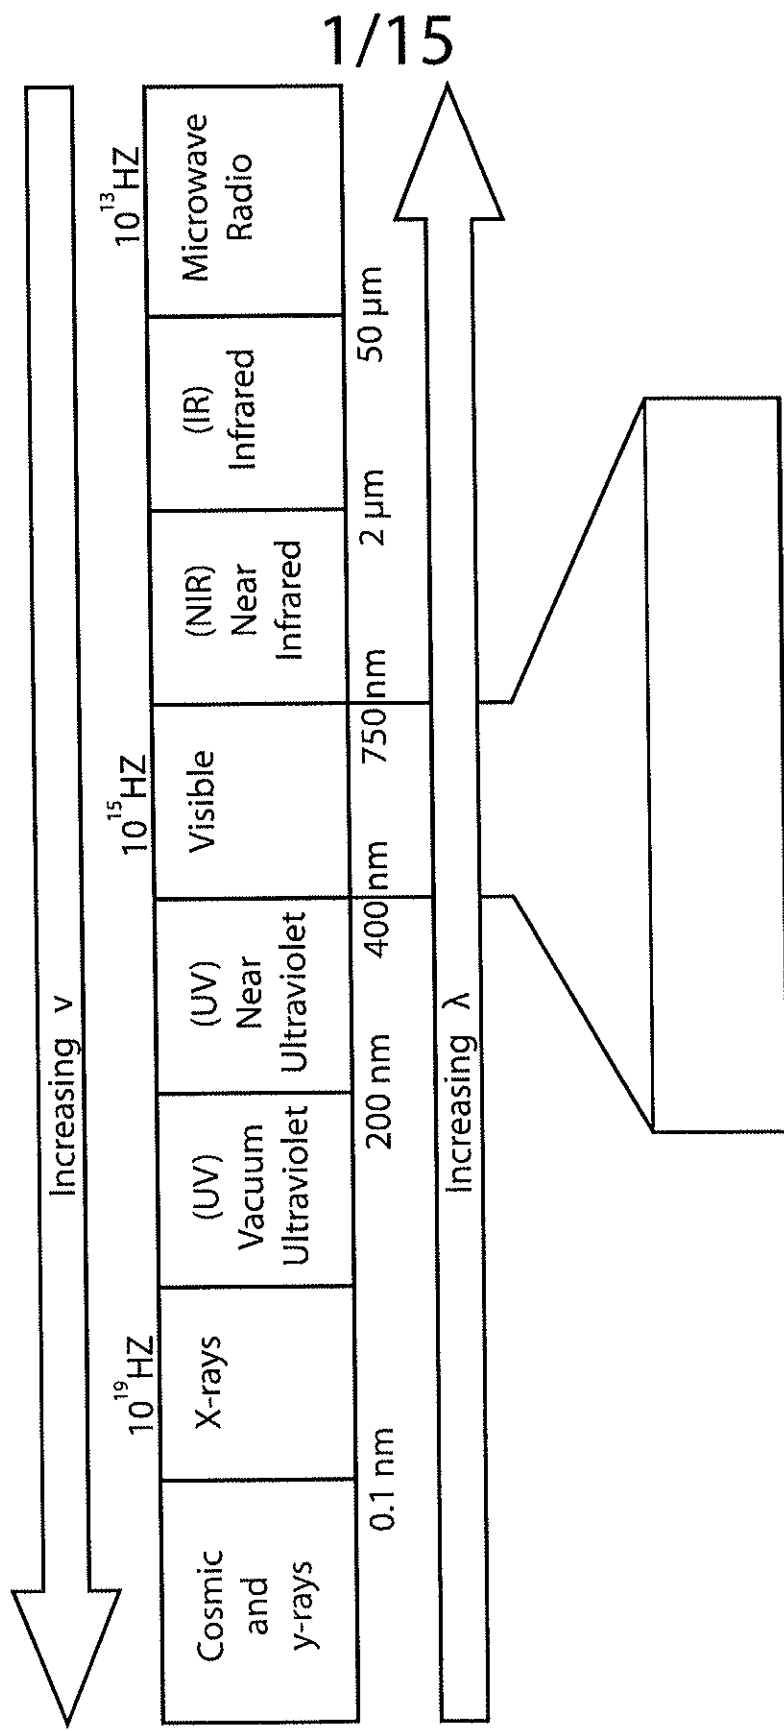


FIG.1

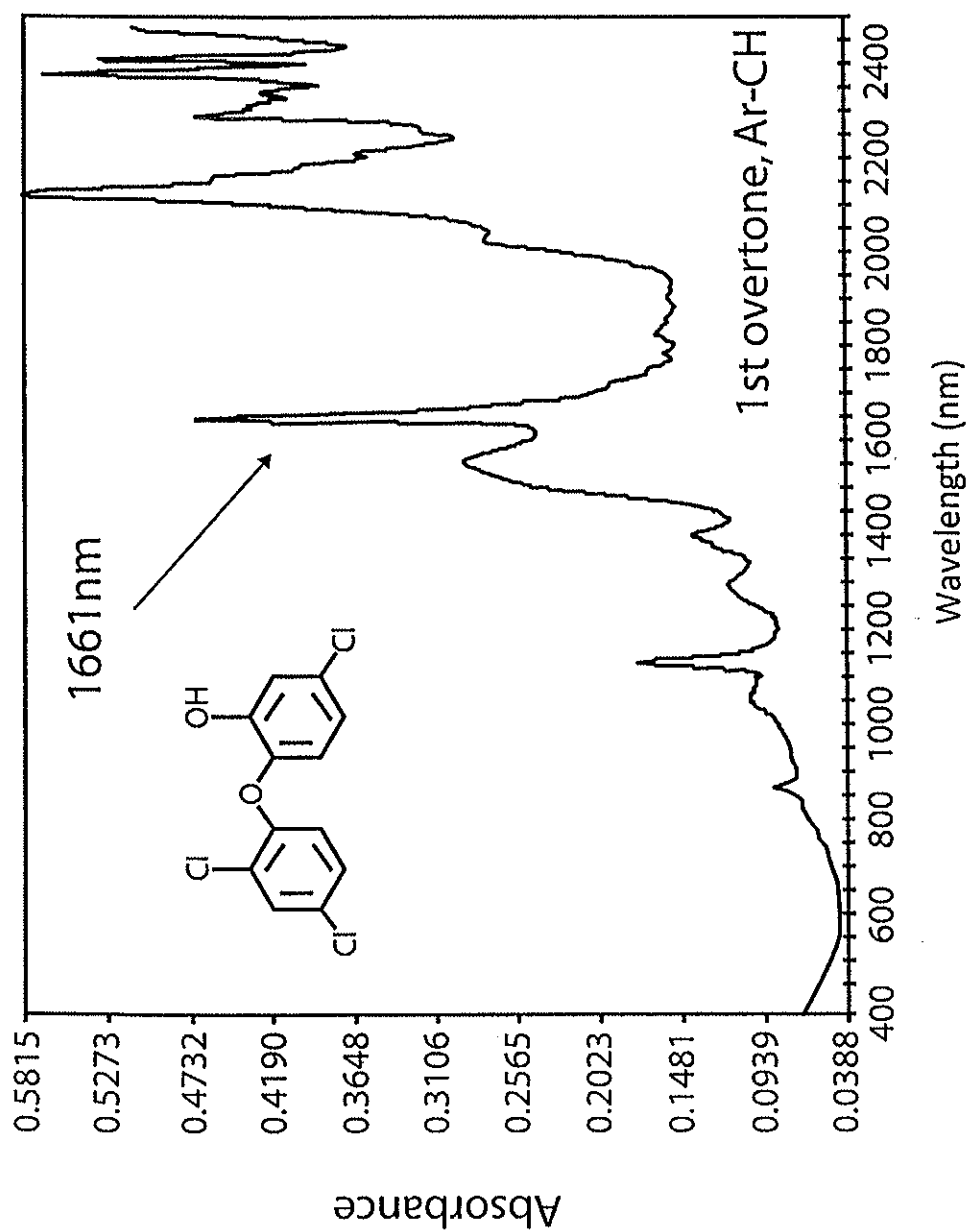


FIG. 2

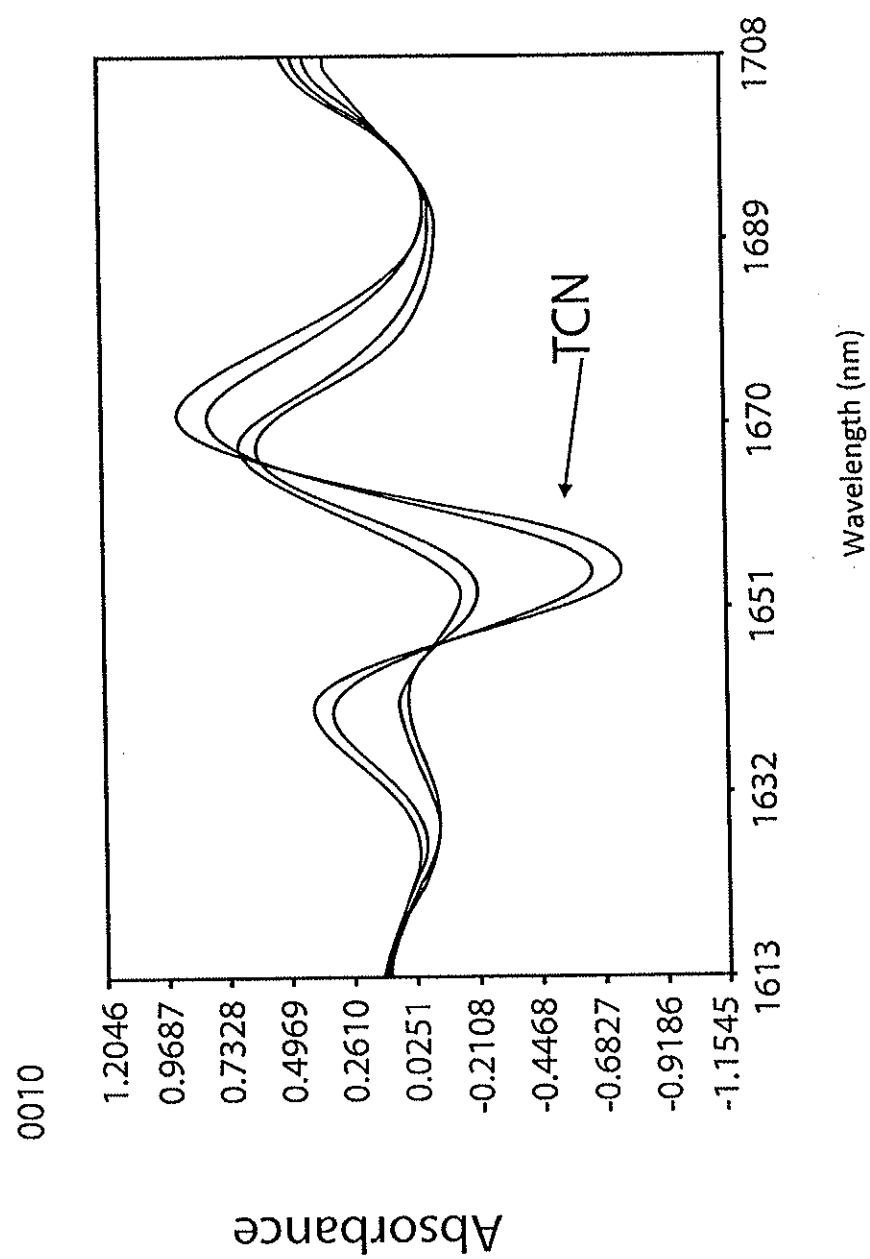


FIG. 3

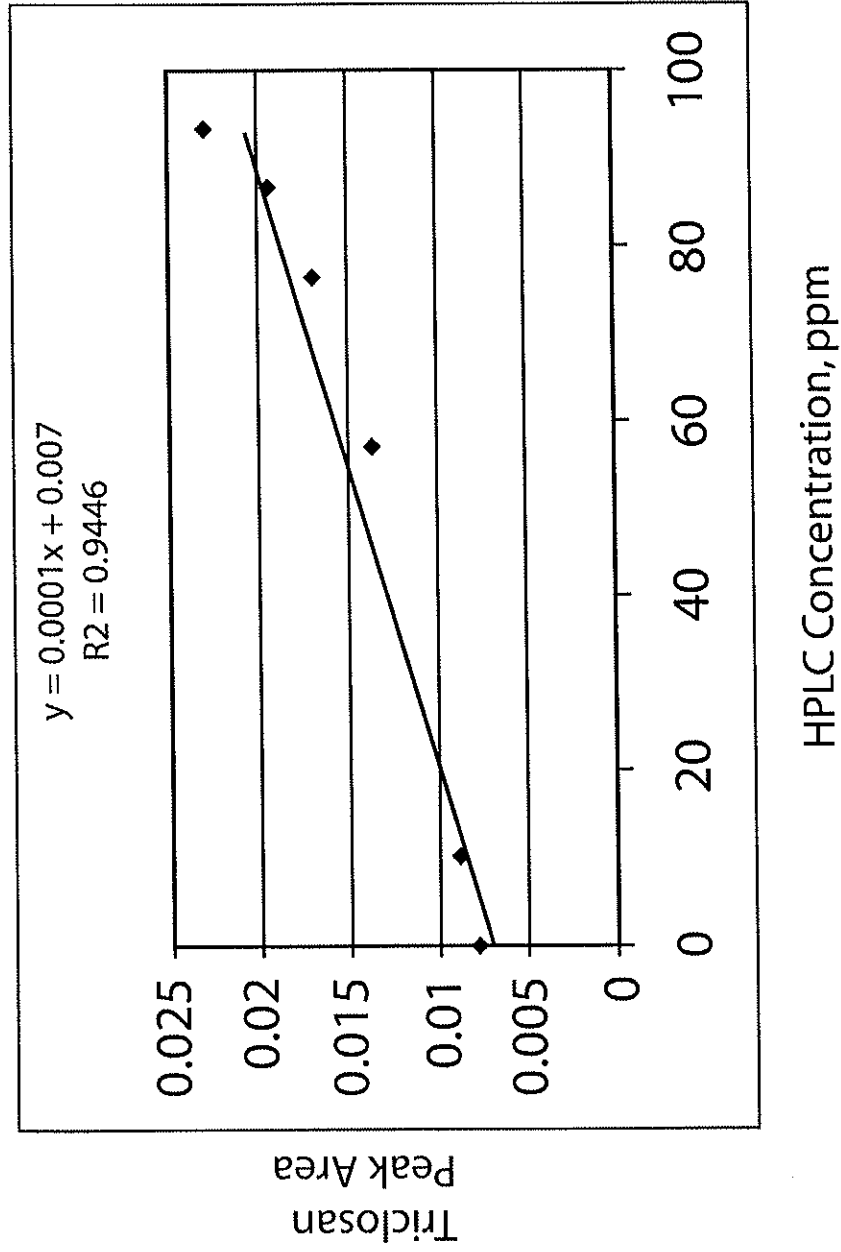


FIG. 4

Sample	Triclosan Deposited, ppm
Delivery System 1, Disk 1	30.7
Delivery System 1, Disk 2	35.0
Delivery System 1, Disk 3	35.1
Delivery System 2, Disk 1	94.3
Delivery System 2, Disk 2	80.0
Delivery System 2, Disk 3	85.1

FIG. 5

6/15

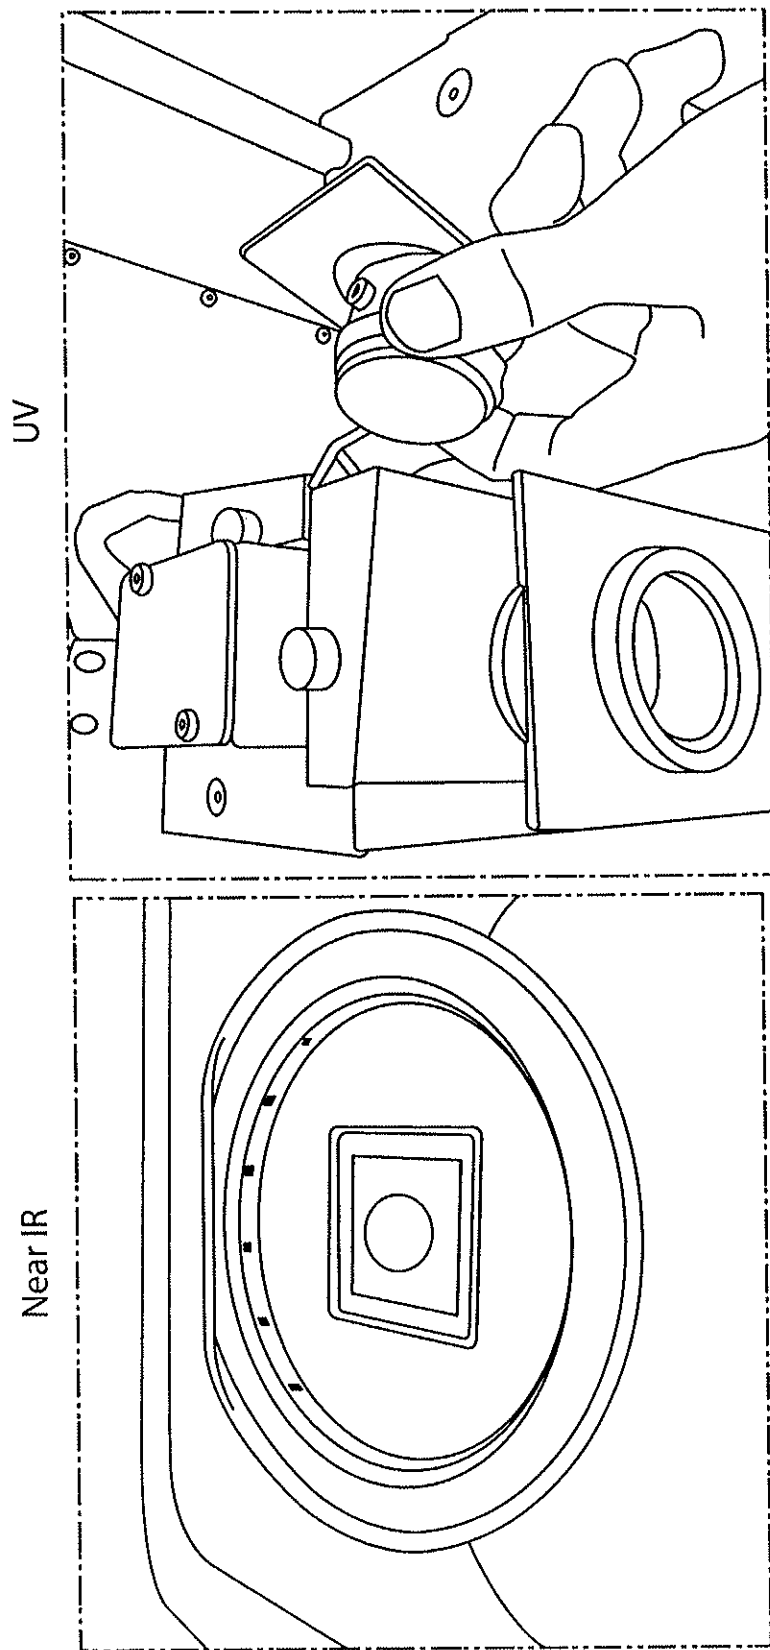


FIG. 6

7/15

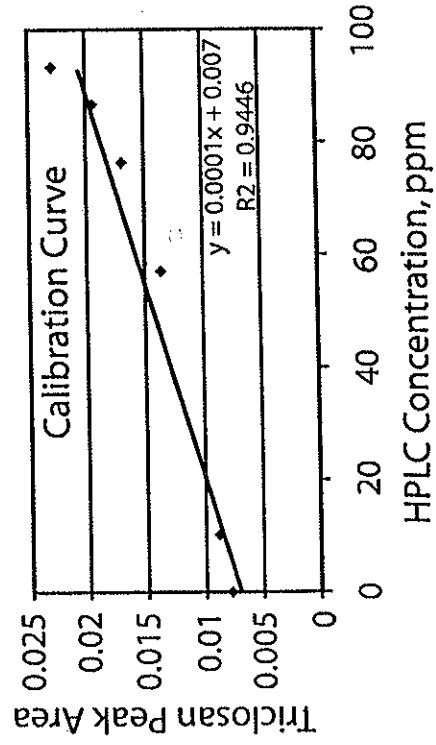
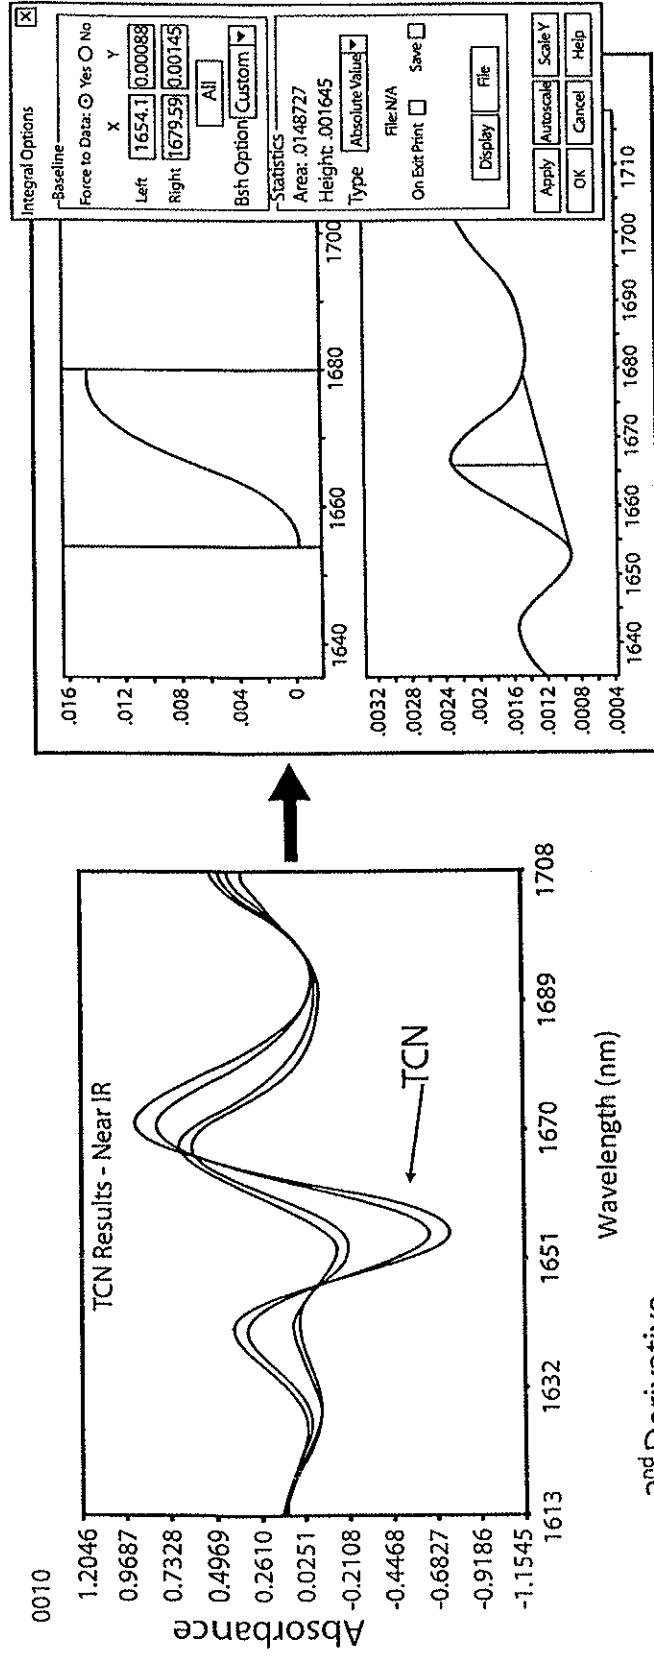


FIG. 7




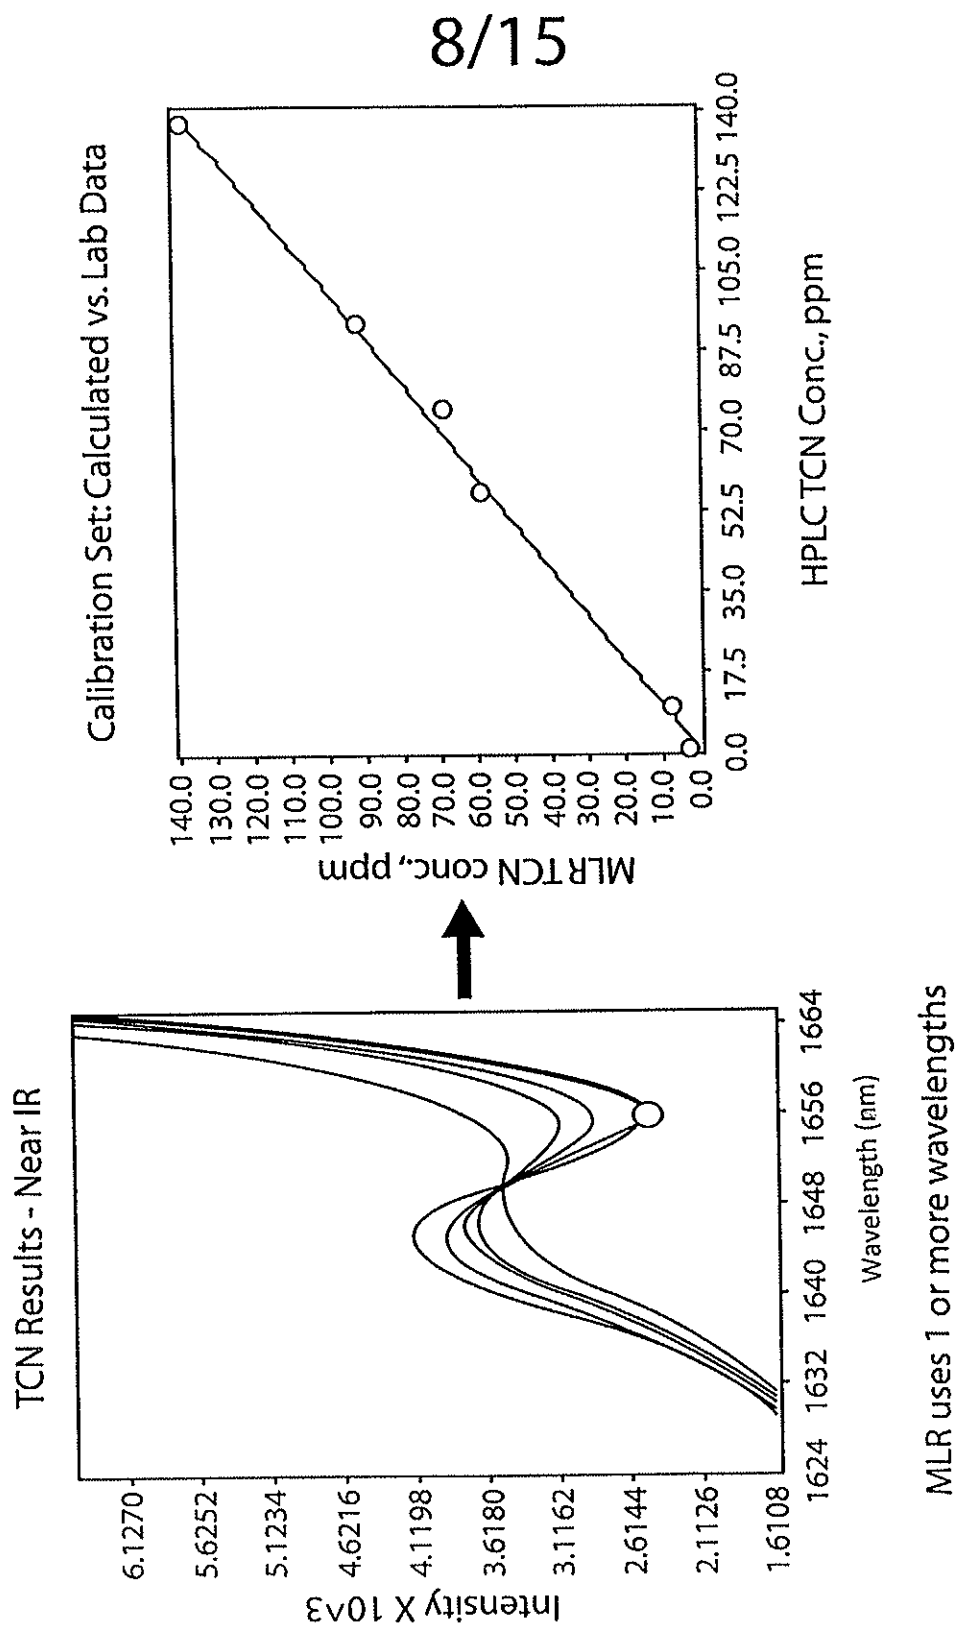


FIG. 8

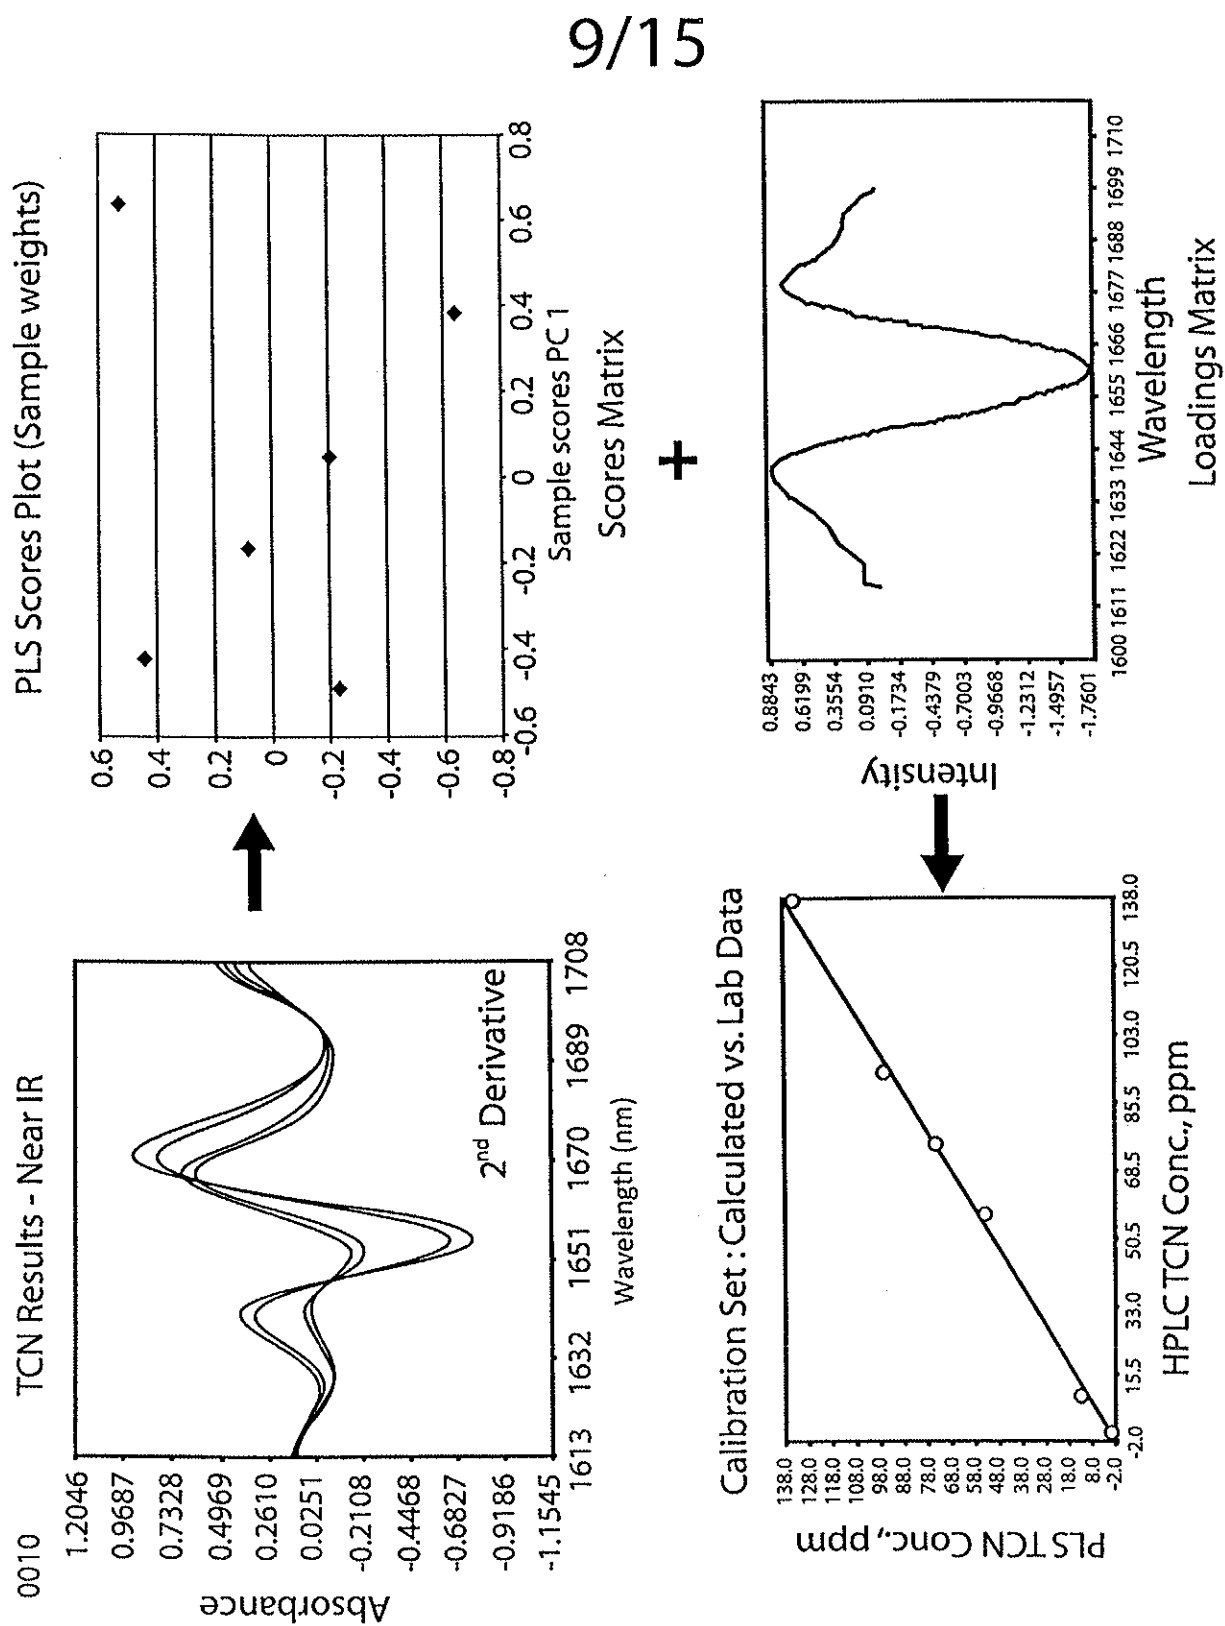


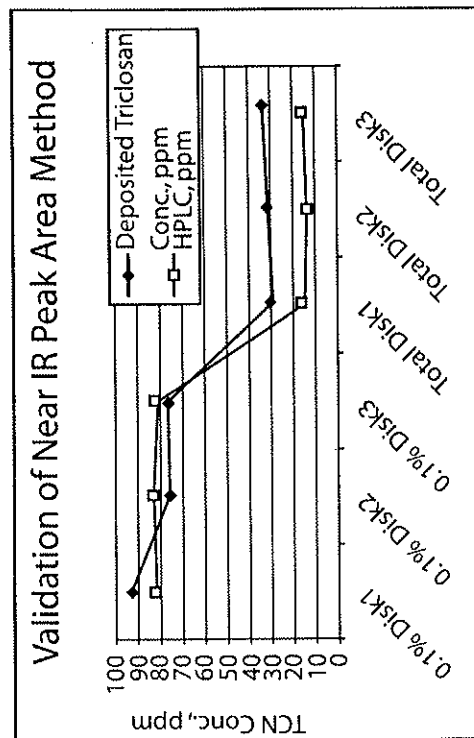

Peak Area SEP ± 10.5 ppm

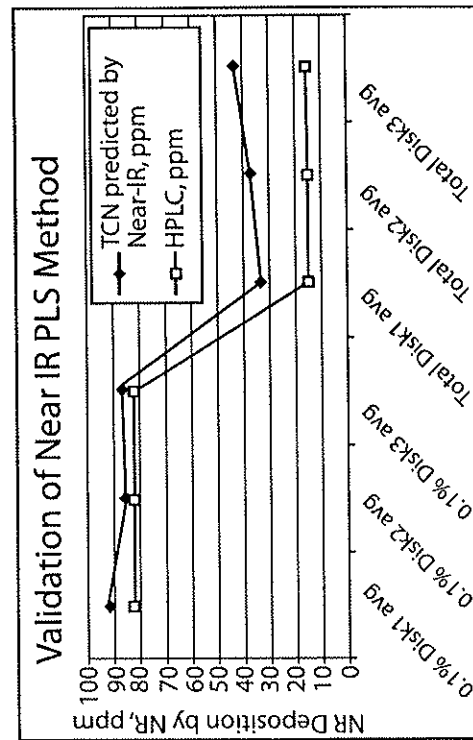


PLS SEP ± 8.6 ppm

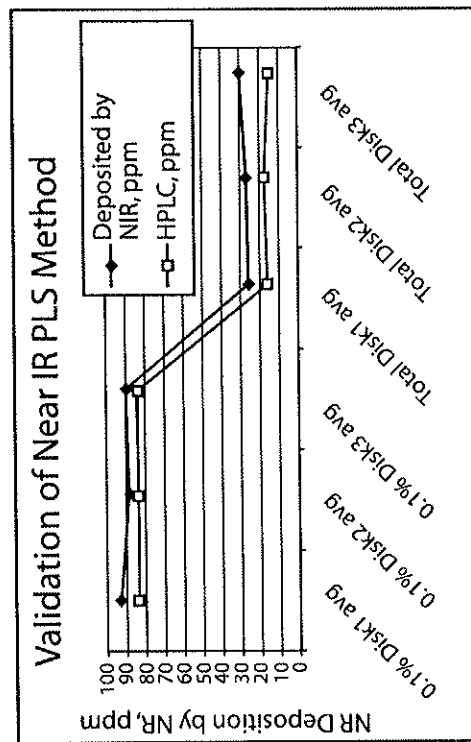

MLR SEP ± 2.8 ppm

FIG. 10

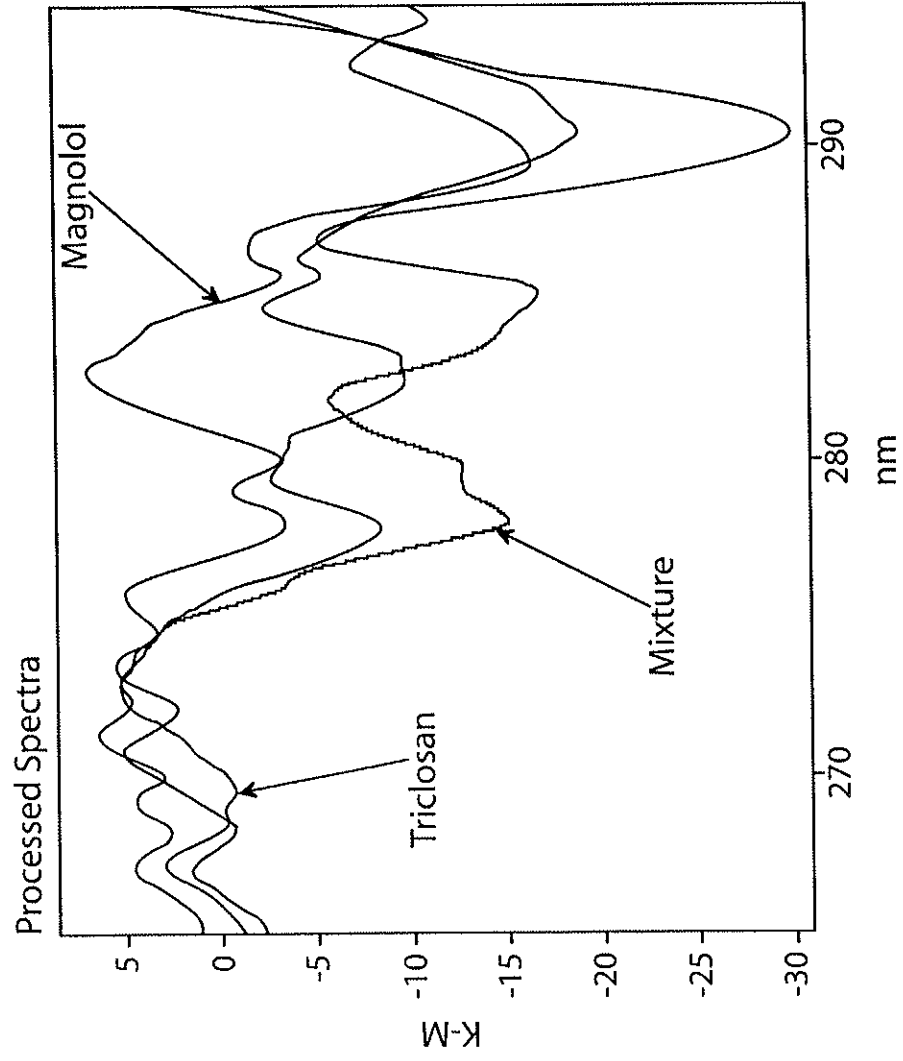

Sample	Triclosan Peak Area	Mixed Active (1:1)	
5 min	4.4 units	52% Triclosan	48% Magnolol
30 min	18.1 units		

11/15

FIG. 11

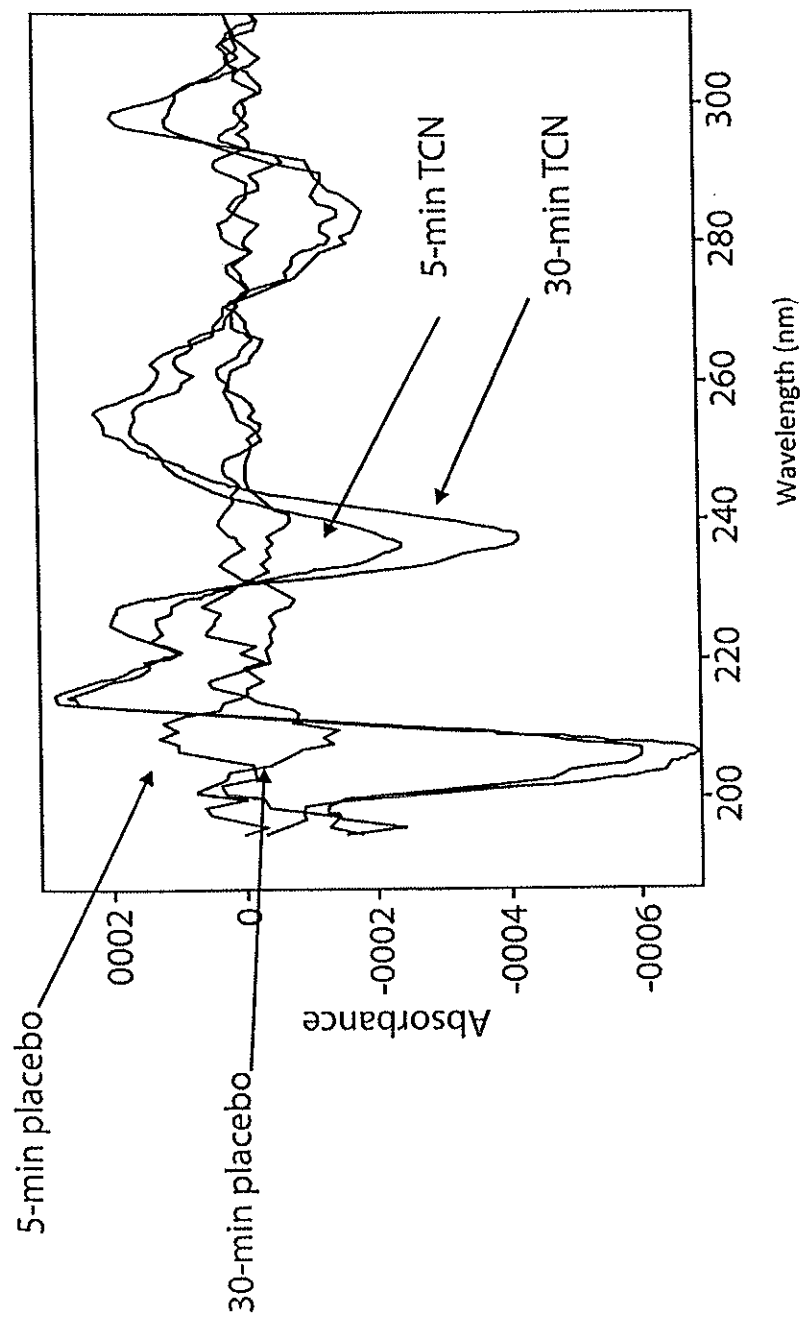


FIG.12

13/15

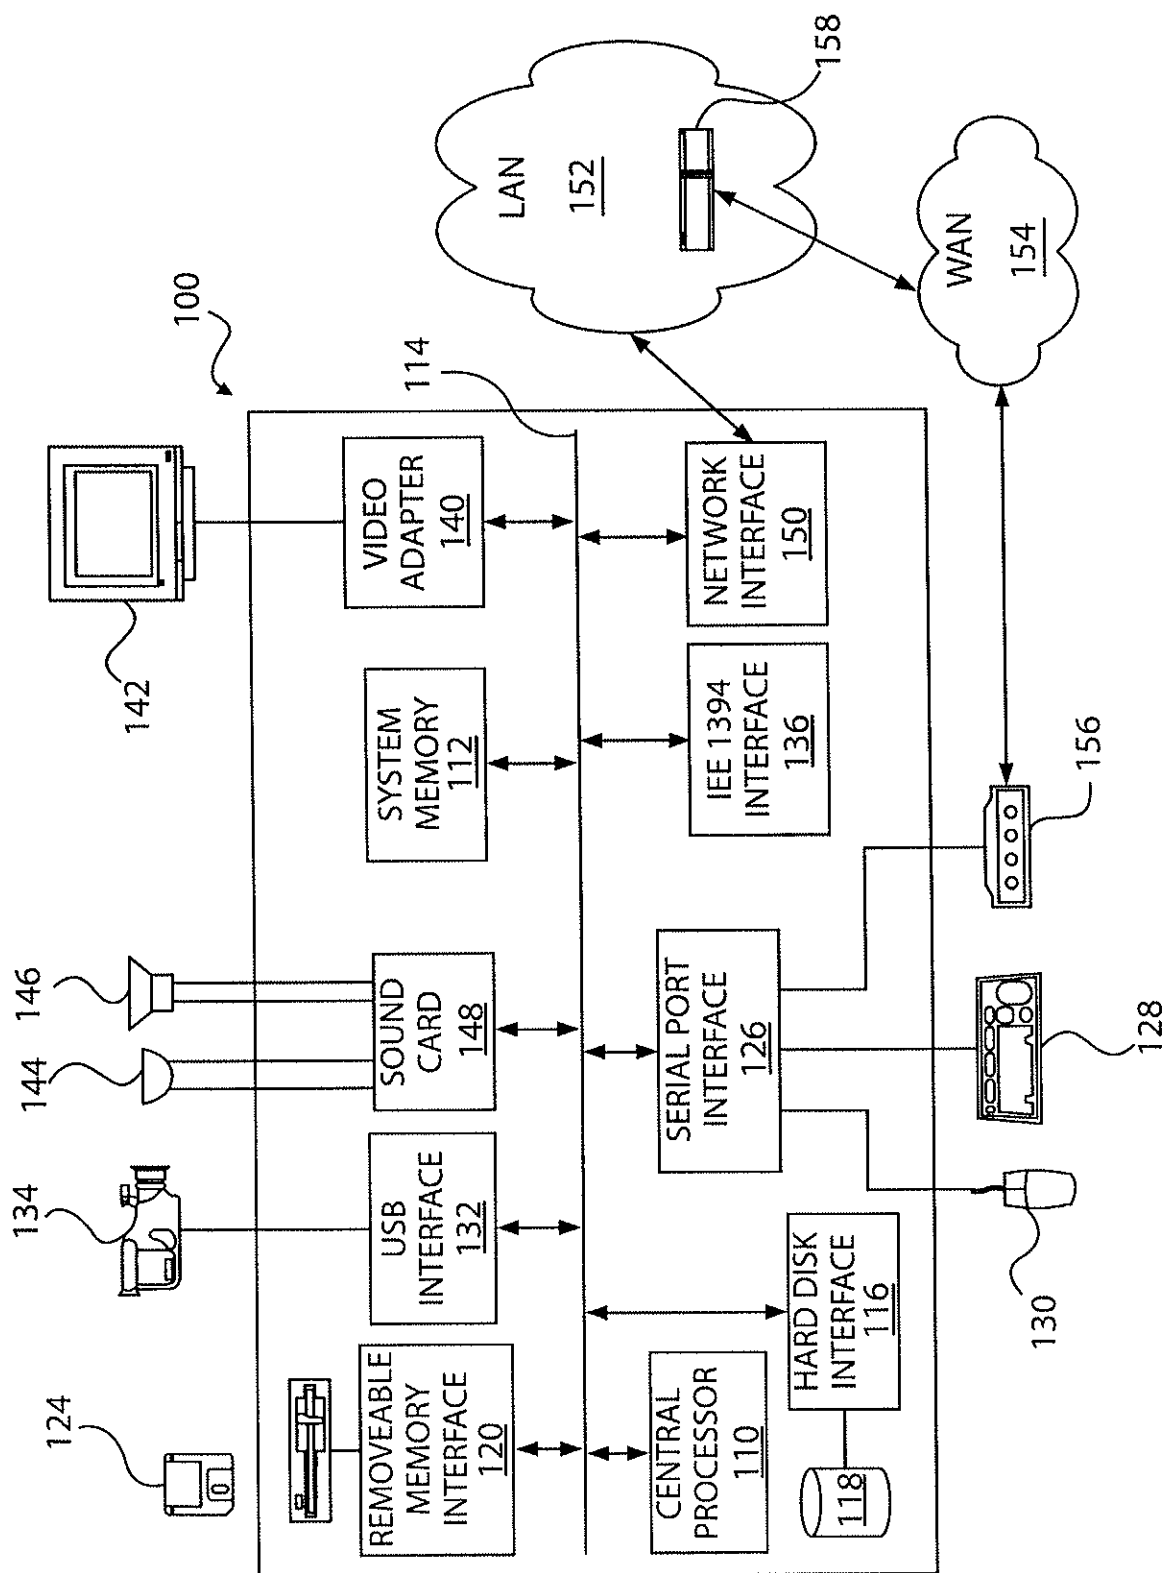


FIG. 13

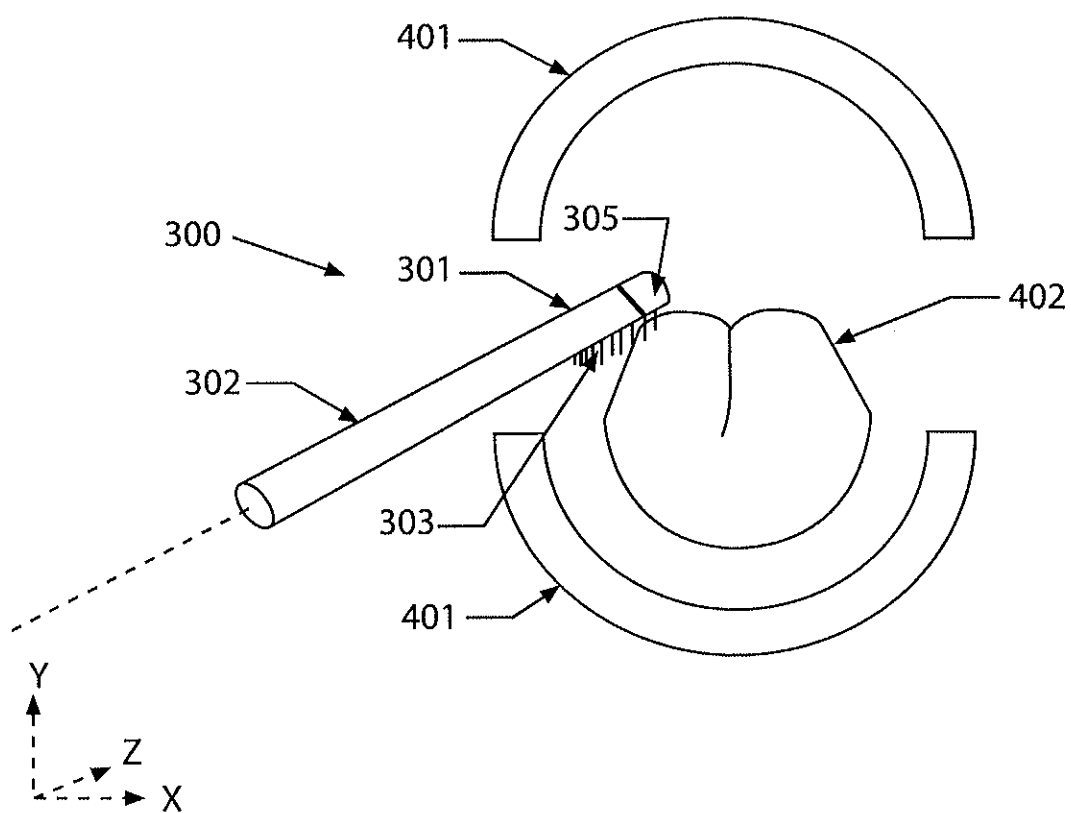


FIG. 14

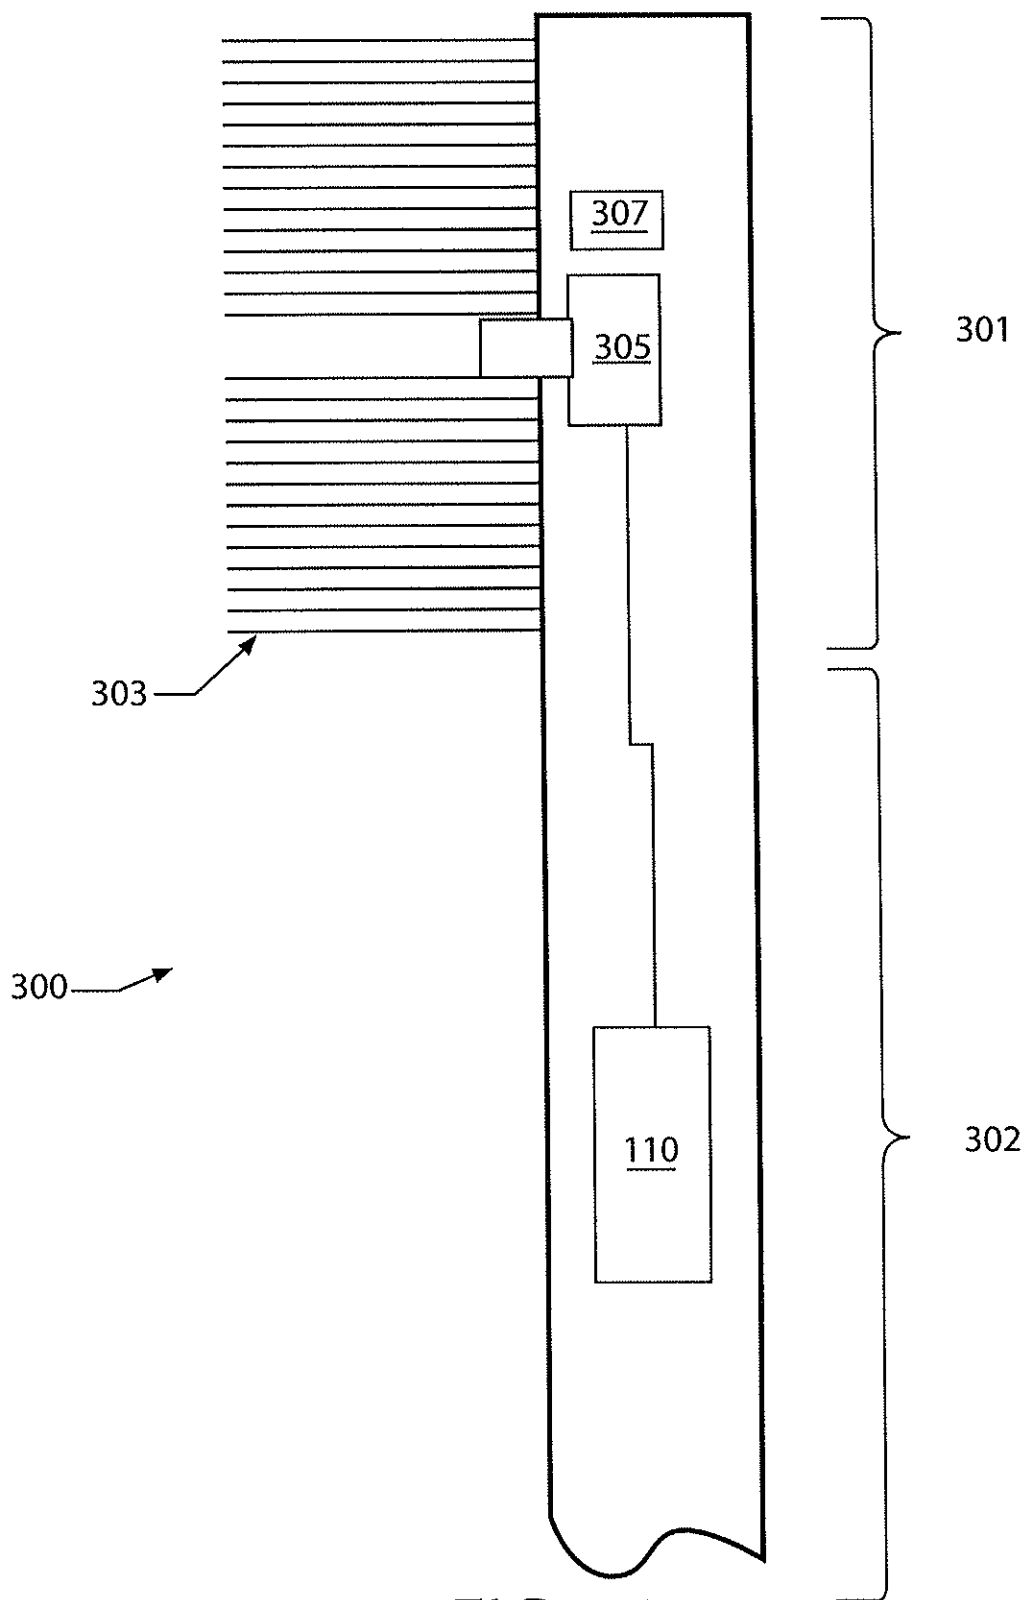


FIG. 15