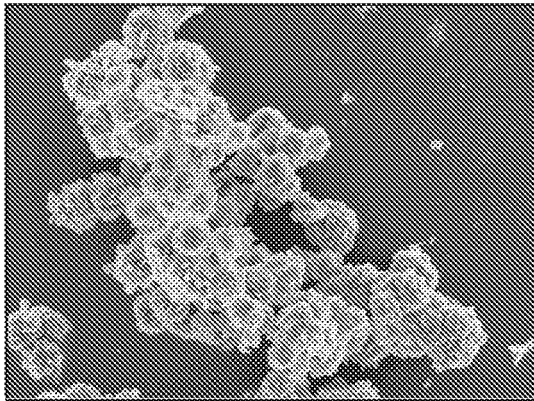
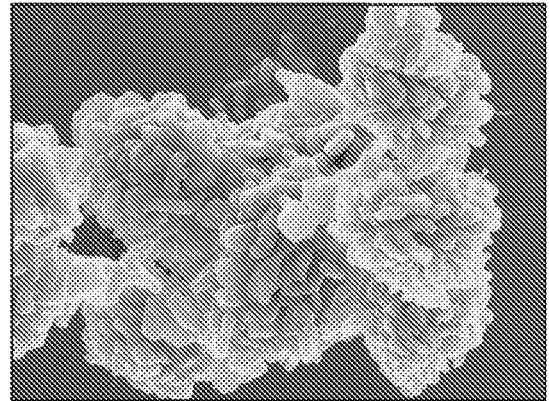


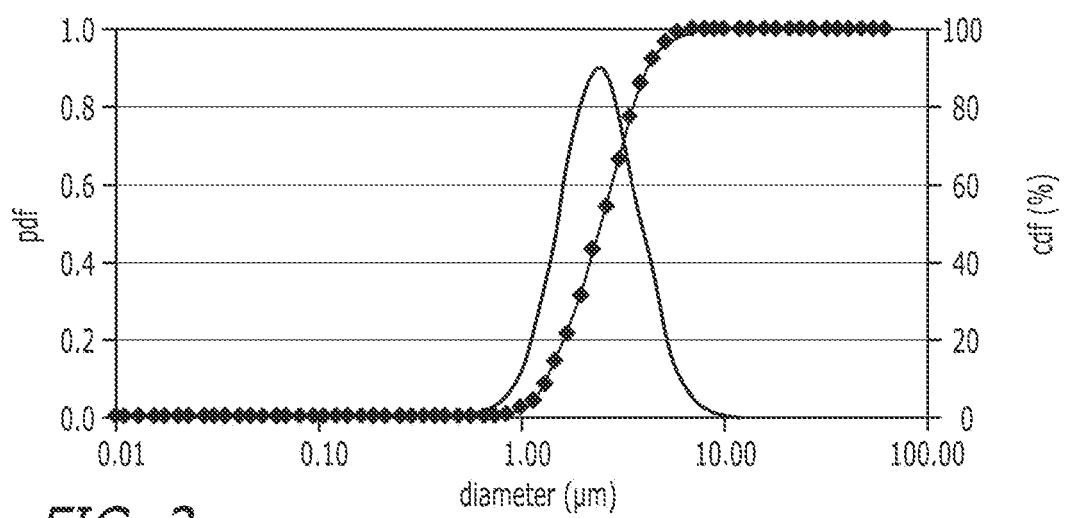
1/7

*FIG. 1A*

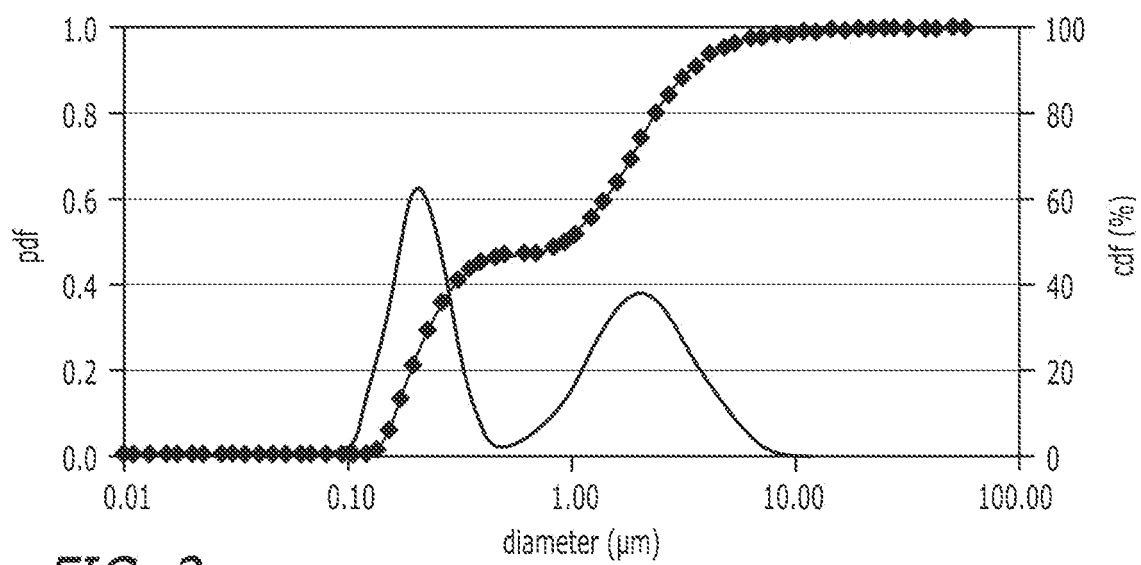
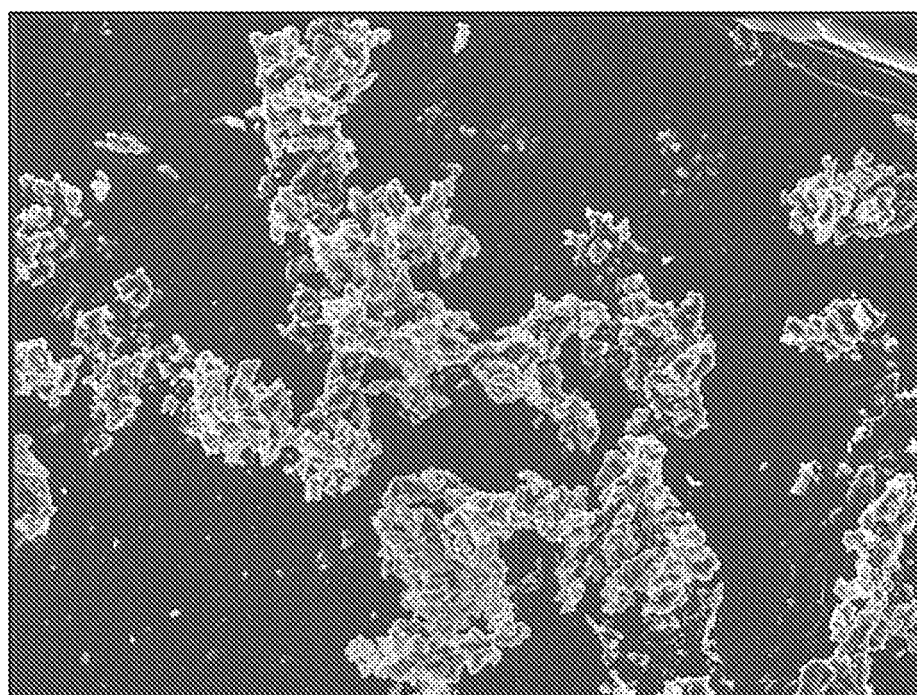
5 μm

*FIG. 1B*

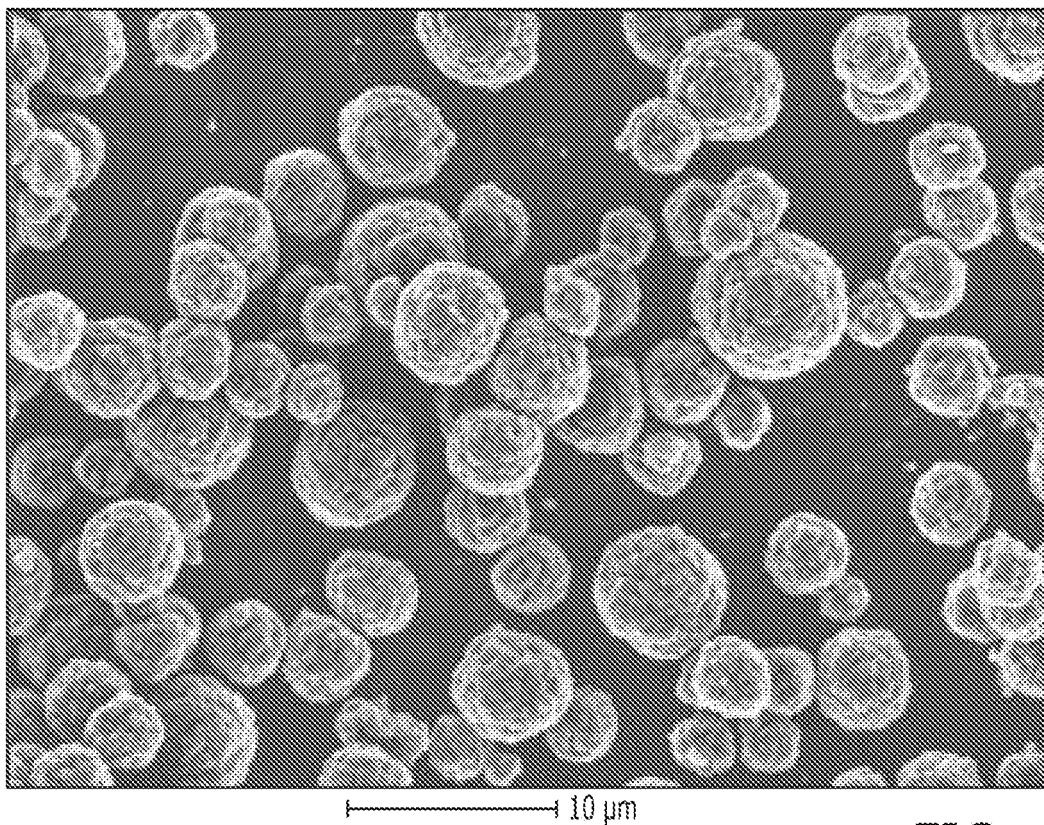
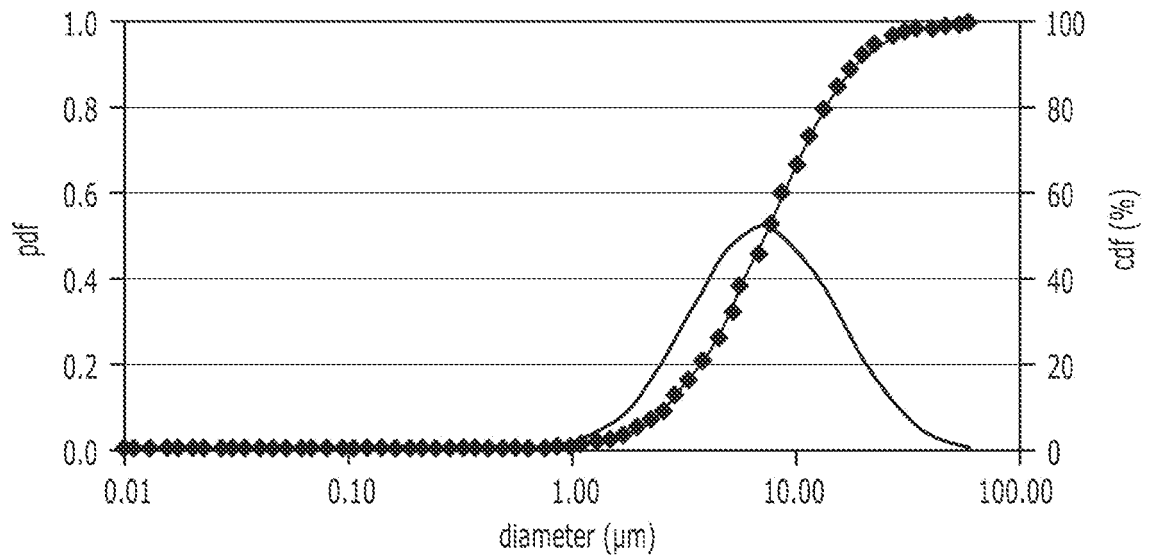
1 μm

*FIG. 2*

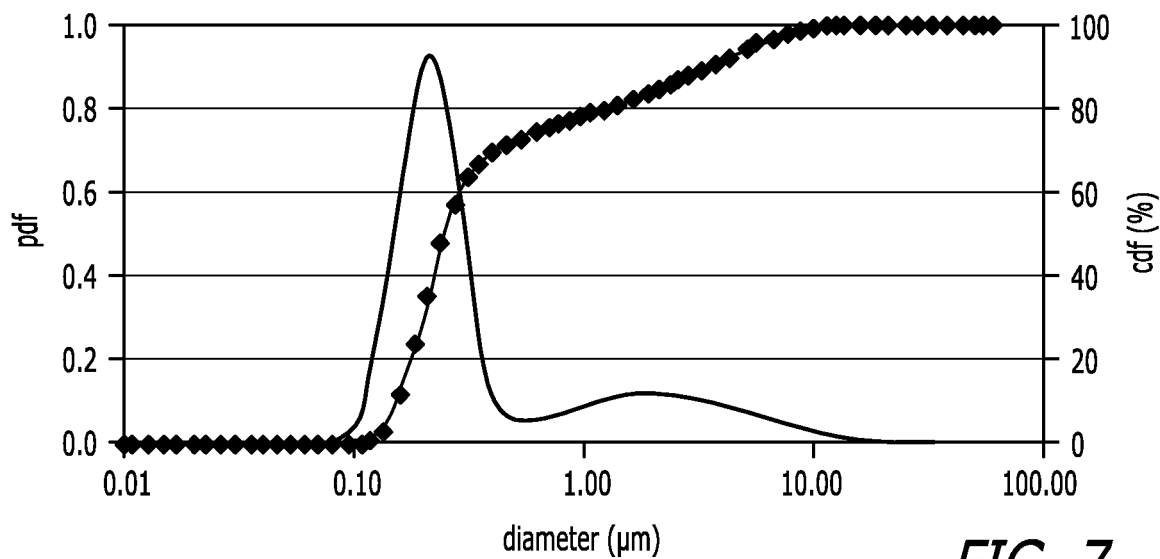
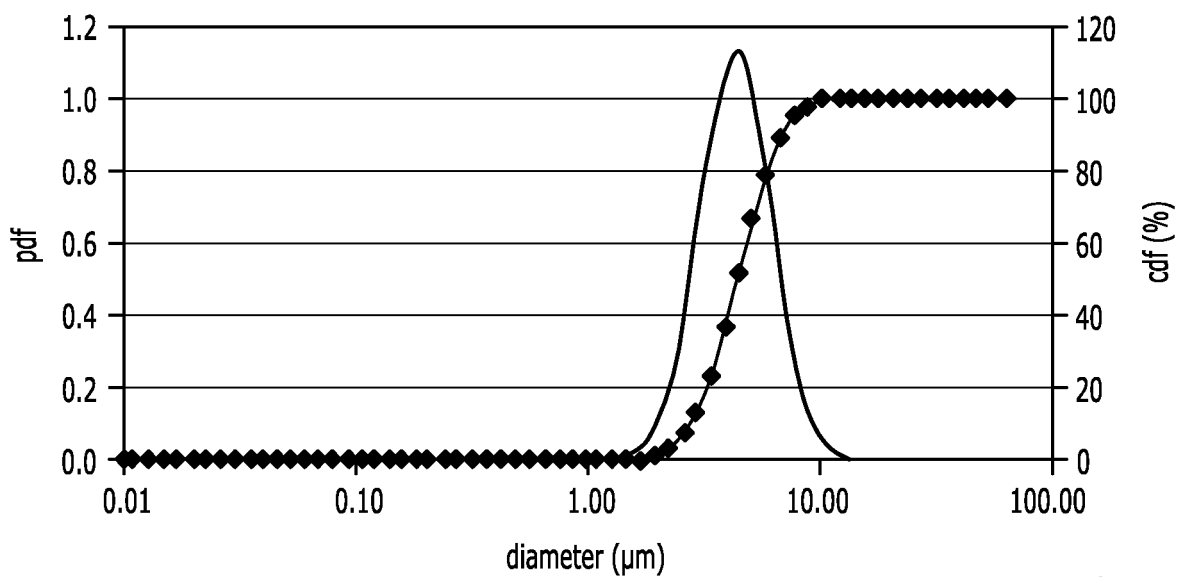
2/7

*FIG. 3**FIG. 4*

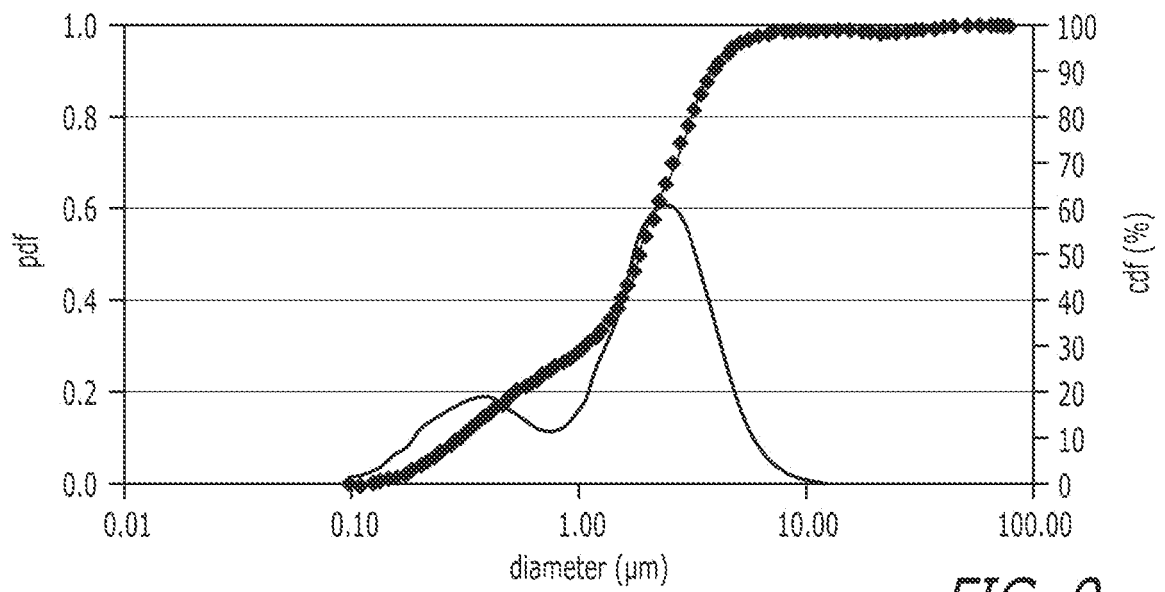
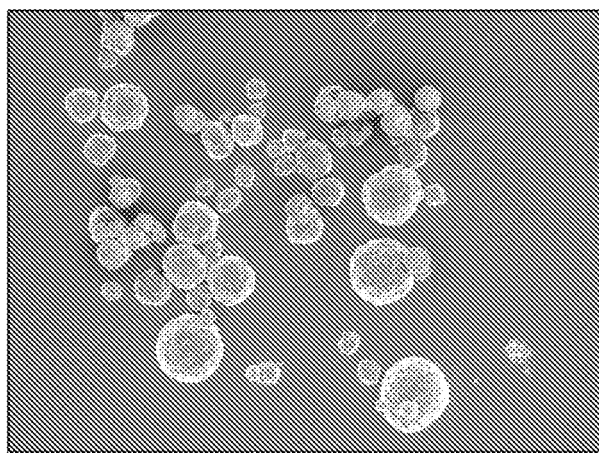
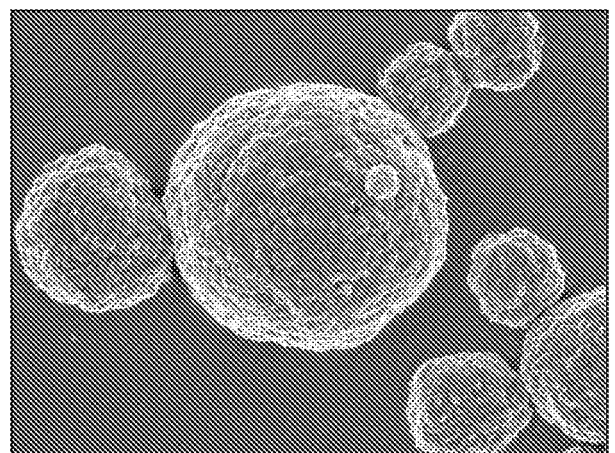
3/7

*FIG. 5**FIG. 6*

4/7

*FIG. 7**FIG. 8*

5/7

*FIG. 9**FIG. 10A**FIG. 10B*

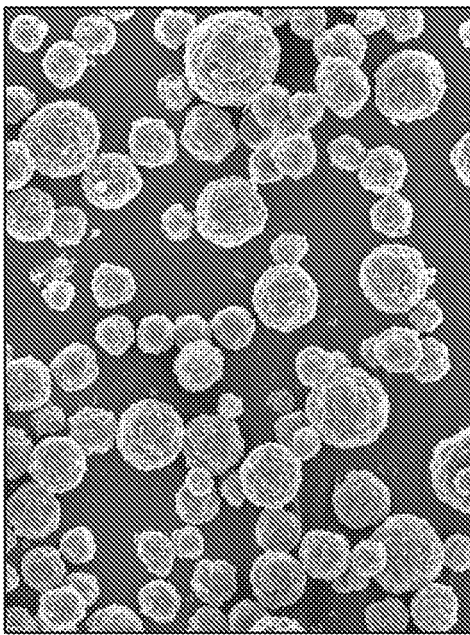


FIG. 11A

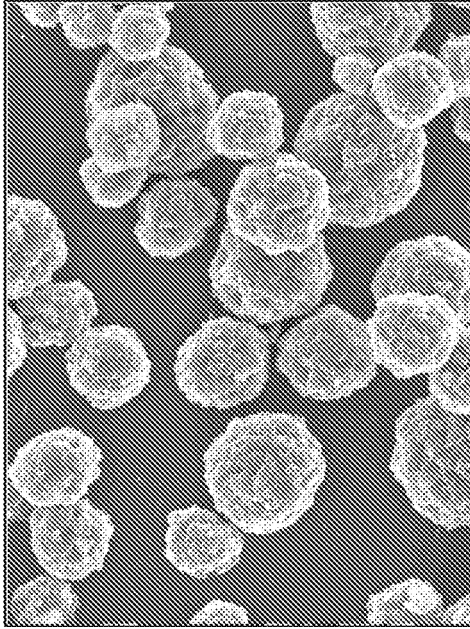


FIG. 11B

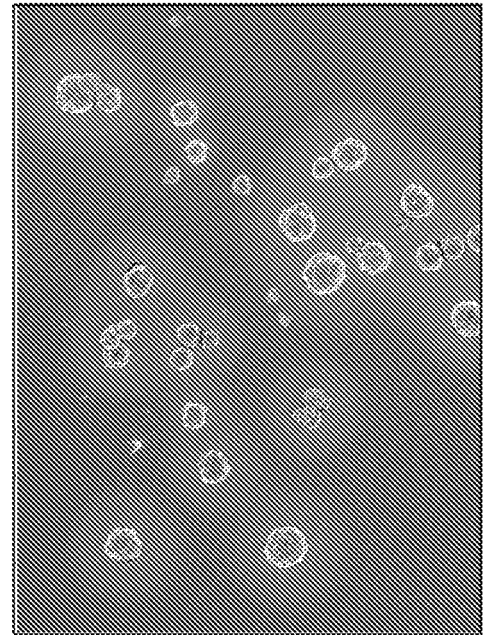


FIG. 12A

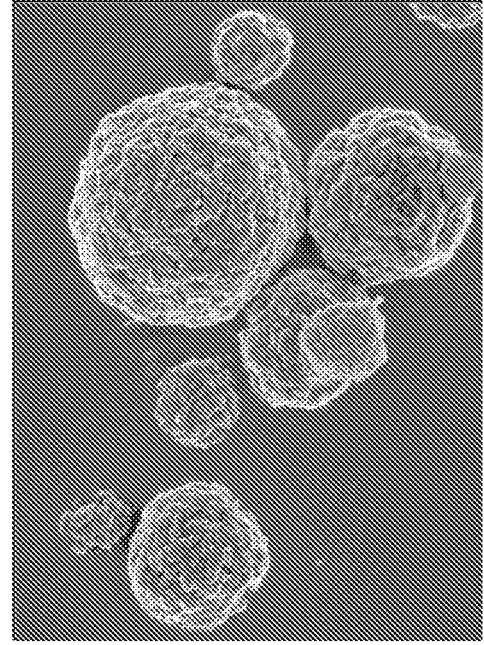
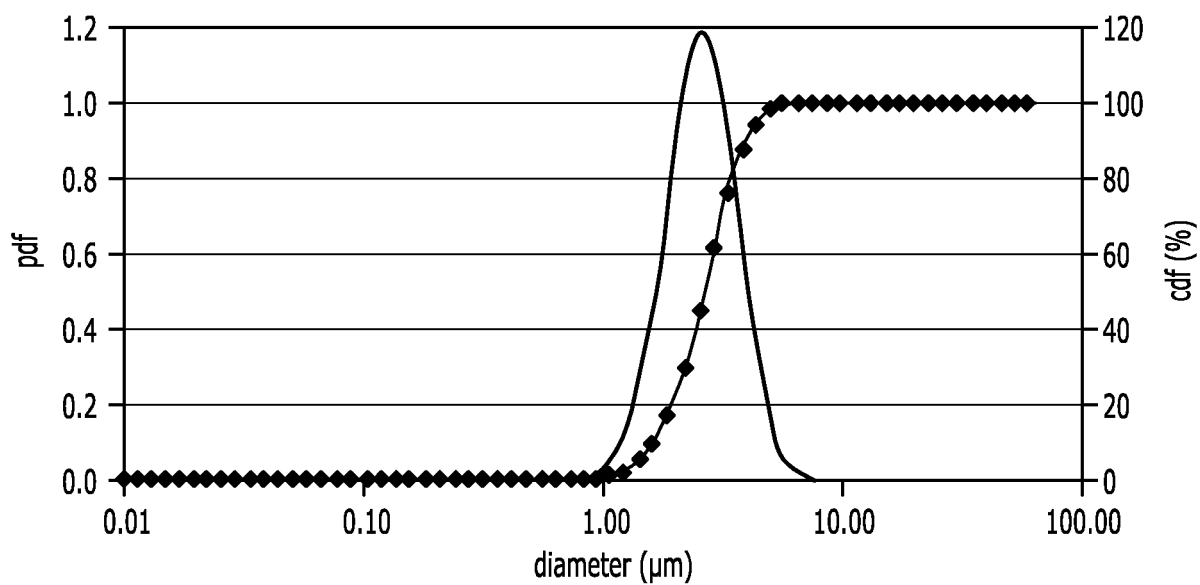
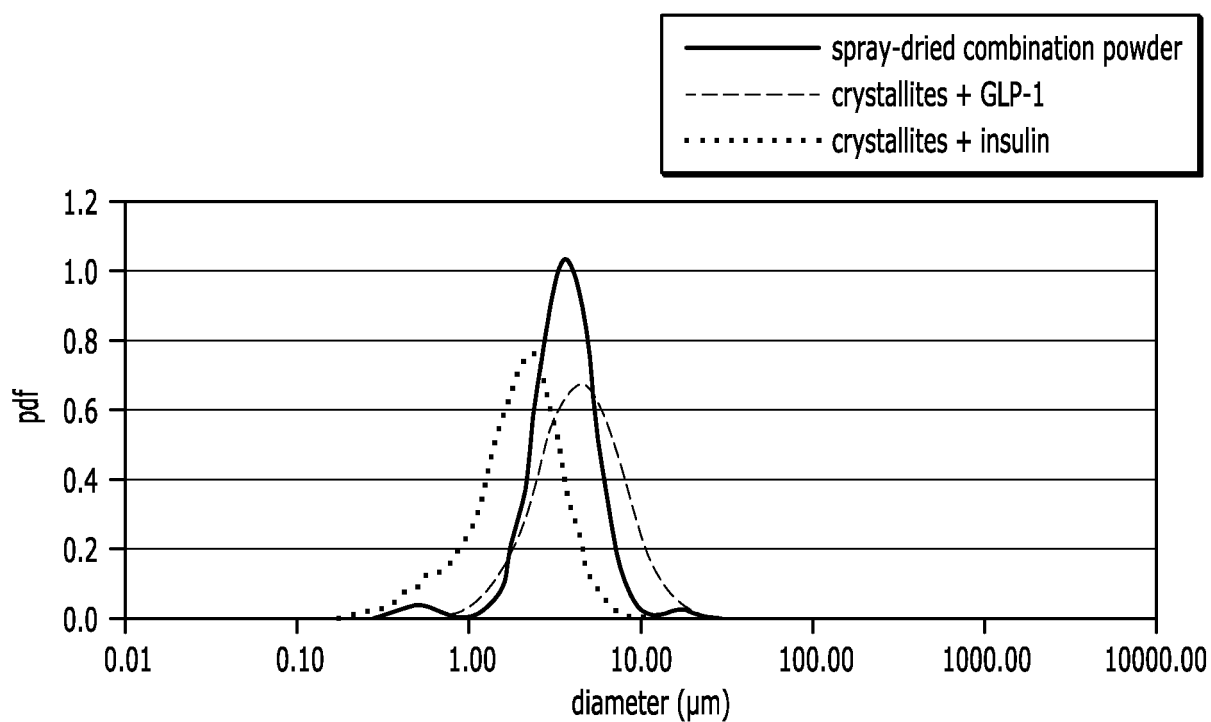


FIG. 12B

7/7

*FIG. 13**FIG. 14*