



- (51) **International Patent Classification:**
A61B 17/22 (2006.01) *A61B 17/00* (2006.01)
- (21) **International Application Number:**
PCT/US2024/052530
- (22) **International Filing Date:**
23 October 2024 (23.10.2024)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**
63/592,502 23 October 2023 (23.10.2023) US
18/923,312 22 October 2024 (22.10.2024) US
- (71) **Applicant: SHOCKWAVE MEDICAL, INC.** [US/US];
5403 Betsy Ross Drive, Santa Clara, California 95054 (US).
- (72) **Inventors: VO, Khanh;** c/o Shockwave Medical, Inc.,
5403 Betsy Ross Drive, Santa Clara, California 95054 (US).
NGUYEN, Tommy; c/o Shockwave Medical, Inc., 5403
Betsy Ross Drive, Santa Clara, California 95054 (US).
ESTRADA, Raymond Chester; c/o Shockwave Medical,
Inc., 5403 Betsy Ross Drive, Santa Clara, California 95054

- (US). **PHAN, Huy;** c/o Shockwave Medical, Inc., 5403 Betsy
Ross Drive, Santa Clara, California 95054 (US). **KAT-
KUOY, Denny;** c/o Shockwave Medical, Inc., 5403 Betsy
Ross Drive, Santa Clara, California 95054 (US).
- (74) **Agent: POLITO, Lea C.** et al.; Morrison & Foerster LLP,
2100 L Street, NW, Suite 900, Washington, District of Co-
lumbia 20037 (US).
- (81) **Designated States** (*unless otherwise indicated, for every
kind of national protection available*): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ,
CA, CH, CL, CN, CO, CR, CU, CV, CZ, DE, DJ, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IQ, IR, IS, IT, JM, JO, JP, KE, KG,
KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY,
MA, MD, MG, MK, MN, MU, MW, MX, MY, MZ, NA,
NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO,
RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, ST, SV, SY, TH,
TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, WS,
ZA, ZM, ZW.
- (84) **Designated States** (*unless otherwise indicated, for every
kind of regional protection available*): ARIPO (BW, CV,

(54) **Title:** SHOCK WAVE CATHETER WITH DIFFERENTLY SIZED SHOCK WAVE EMITTERS

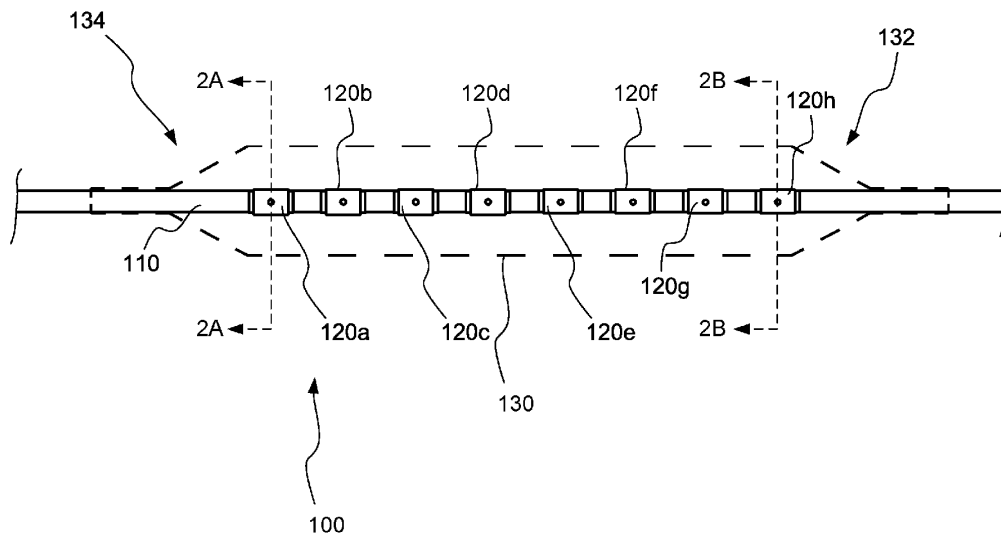


FIG. 1

(57) **Abstract:** A catheter for treating a lesion in a body lumen includes an elongate member, an enclosure, and shock wave emitters enclosed by the enclosure. At least one of the shock wave emitters has a different size than at least one of the other emitters. Providing a smaller shock wave emitter at a distal end of the catheter can help make the catheter more navigable through the body lumen.

[Continued on next page]

GH, GM, KE, LR, LS, MW, MZ, NA, RW, SC, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, ME, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

- with international search report (Art. 21(3))
- with amended claims (Art. 19(1))