

1/6


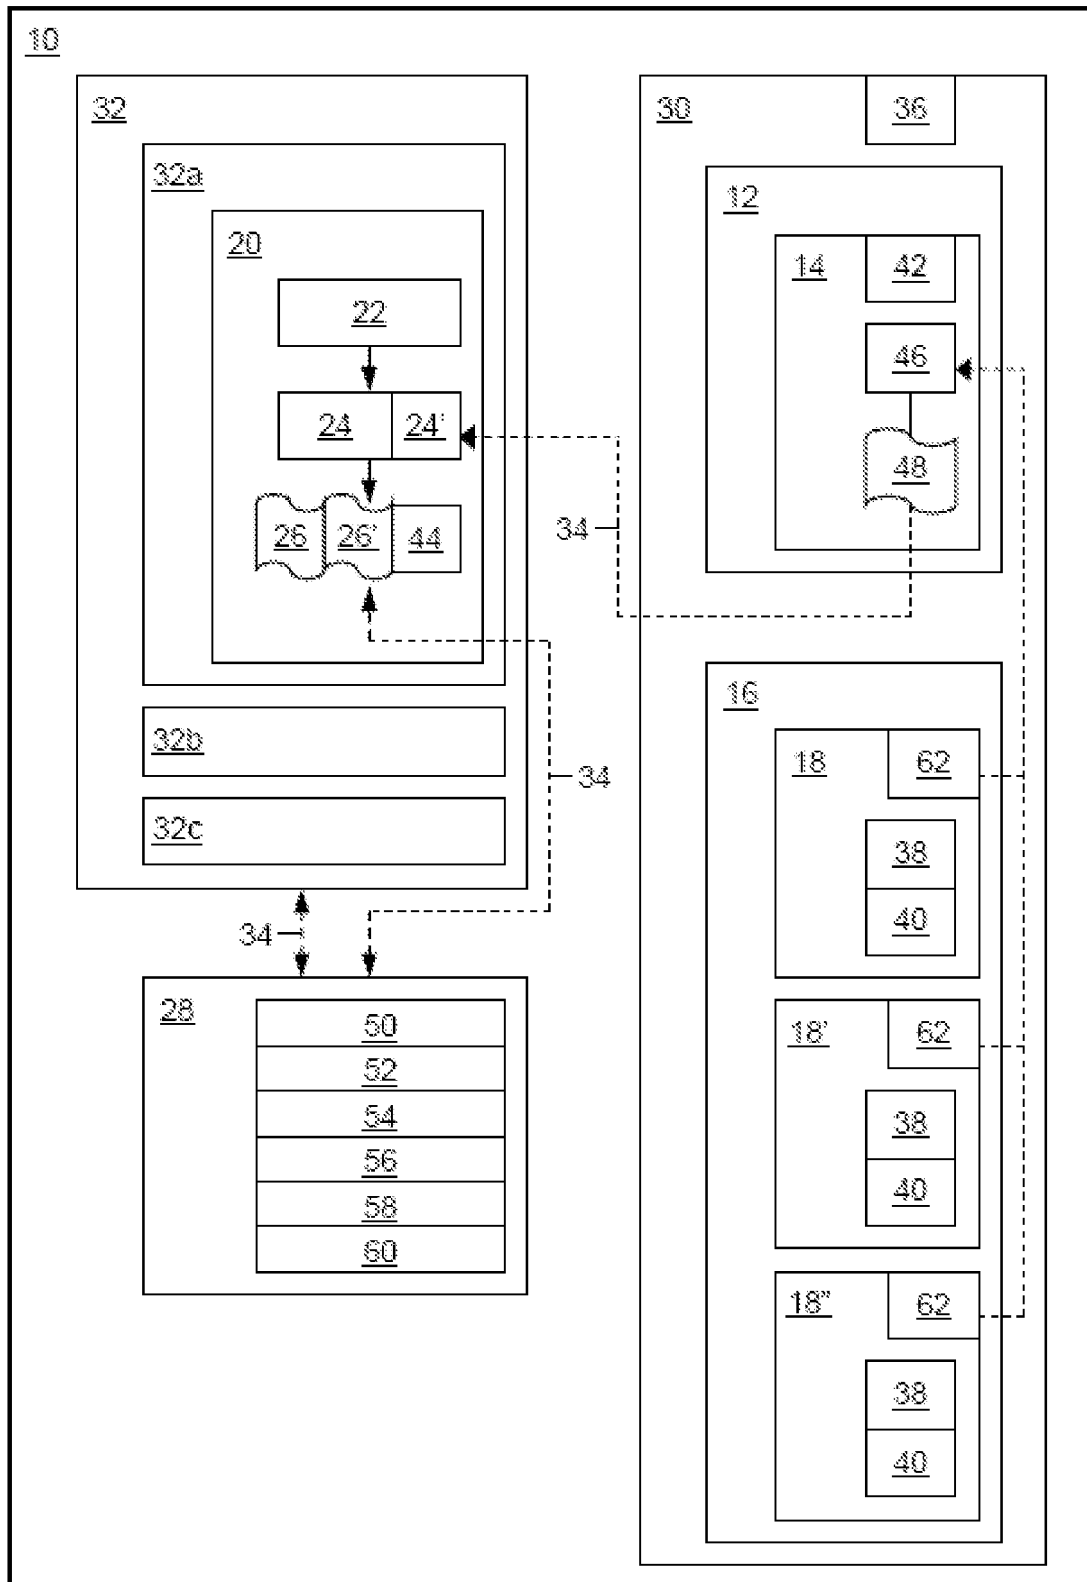


FIG. 1

Step 1 : Select Application

Select the chromatography application in which you are using the selected consumable(s)



☒ Gas Chromatography (GC)

Gas Chromatography (GC)



☐ Liquid Chromatography (LC)

Liquid Chromatography (LC)



☐ ICP

ICP

Detector Type:

☒ MS

☐ ECD

☐ ELCD

☐ NPD

☐ FID

Detector Type:

☐ MS

Detector Type:

☐ MS

Previous

Next

FIG. 2

Step 2 : Application Usage

Please indicate the necessary details to calculate the lifetime of the selected consumable(s)

Gas Chromatography (GC) / MS

Carrier Gas

Helium

Source Gas Quality (%)

99.9999

Gas Delivery System

☒ Bottle ☐ Generator

Usage:

☒ Daily ☐ Weekly ☐ Monthly

Flow

2 L/min.

pressure

5 Bar ☐ Psi

Tubing & Fittings

Material: ☒ Stainless Steel ☐ Brass

Size: ☐ 1/4" ☒ 1/8"

Sample(s). Runtime per sample:

5

30 Minutes

25 Seconds

Previous

Next

FIG. 3

4/6

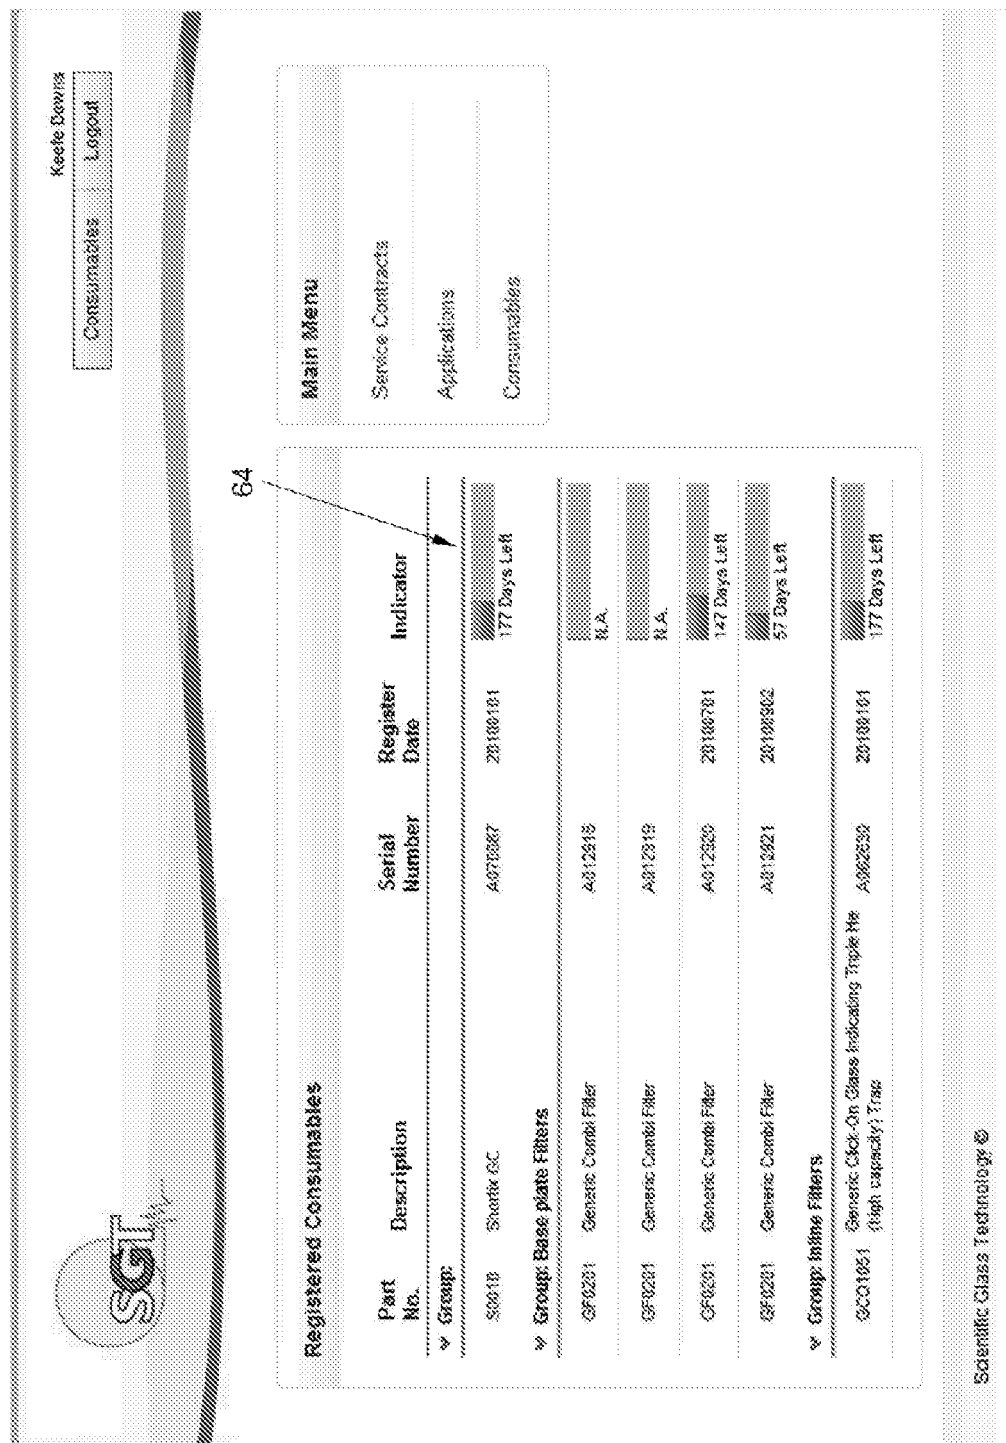


FIG. 4

5/6

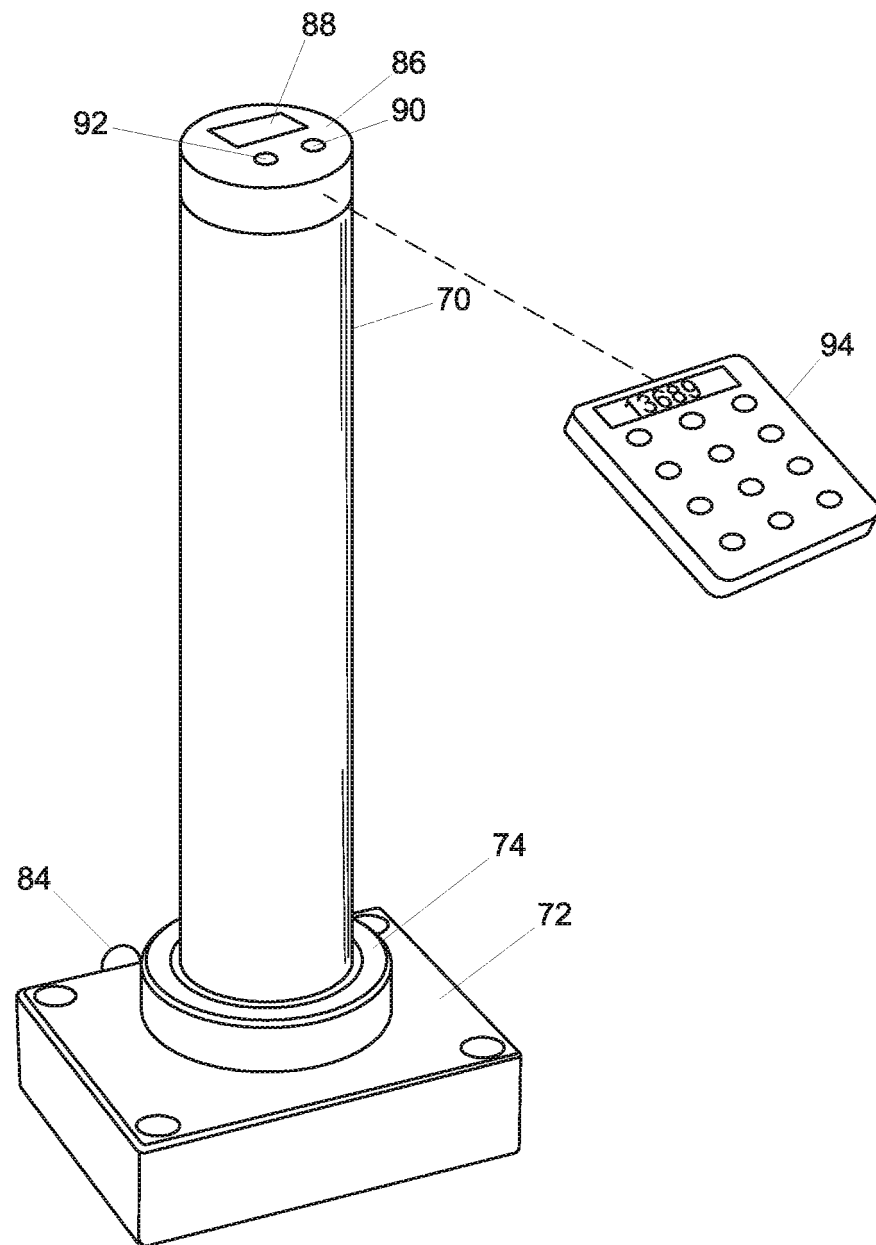


FIG. 5

6/6

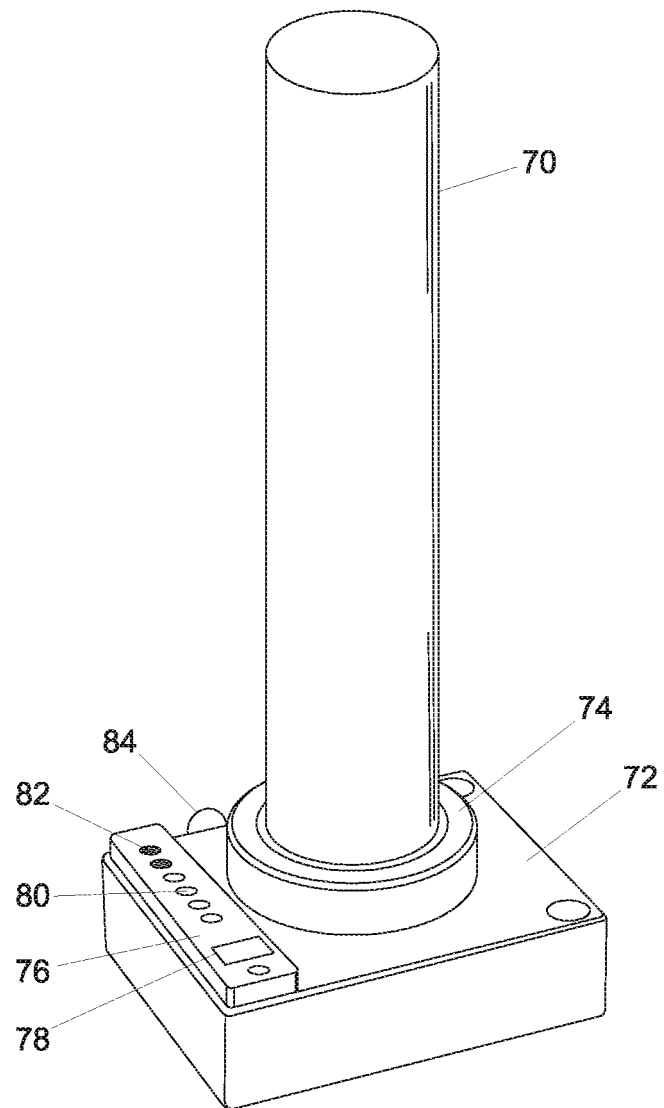


FIG. 6