

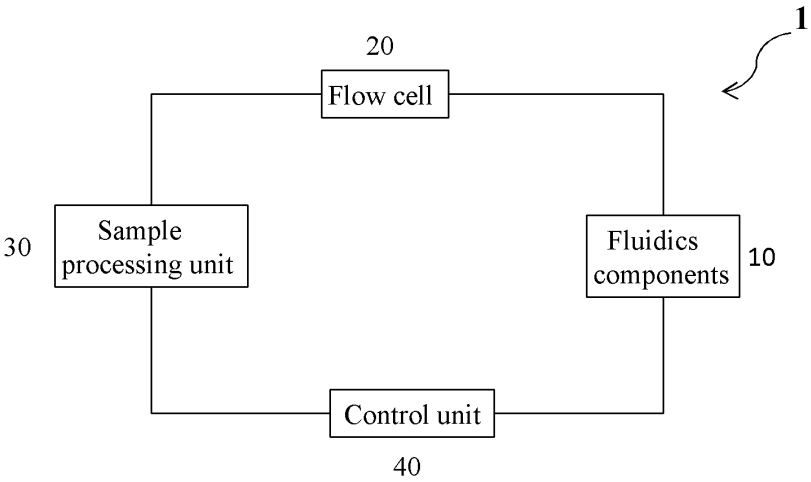


FIG.1

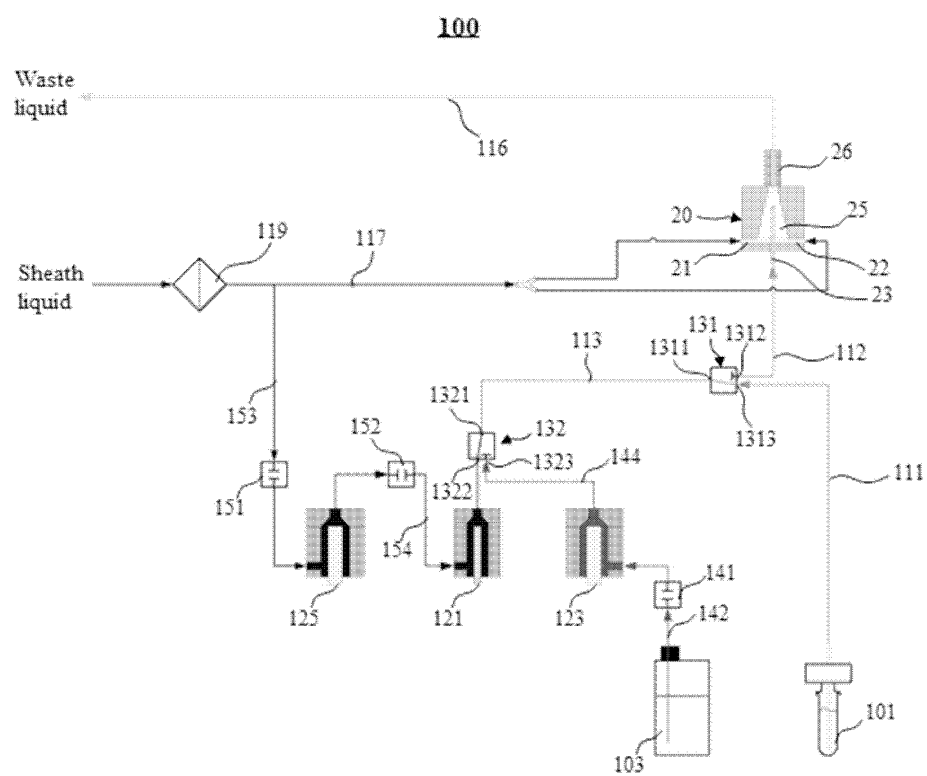


FIG.2

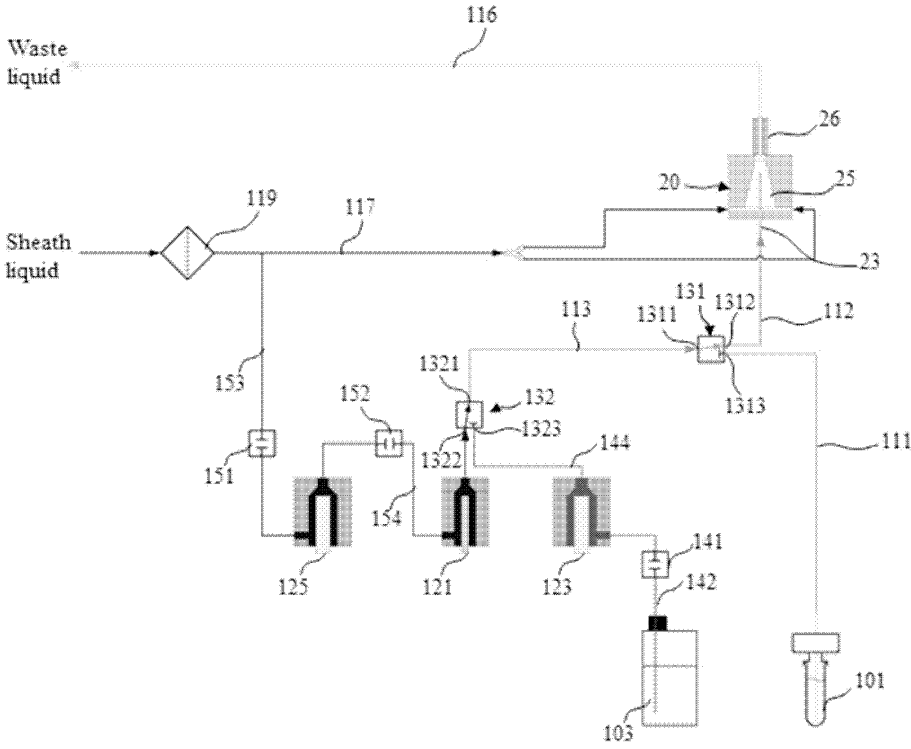


FIG.3

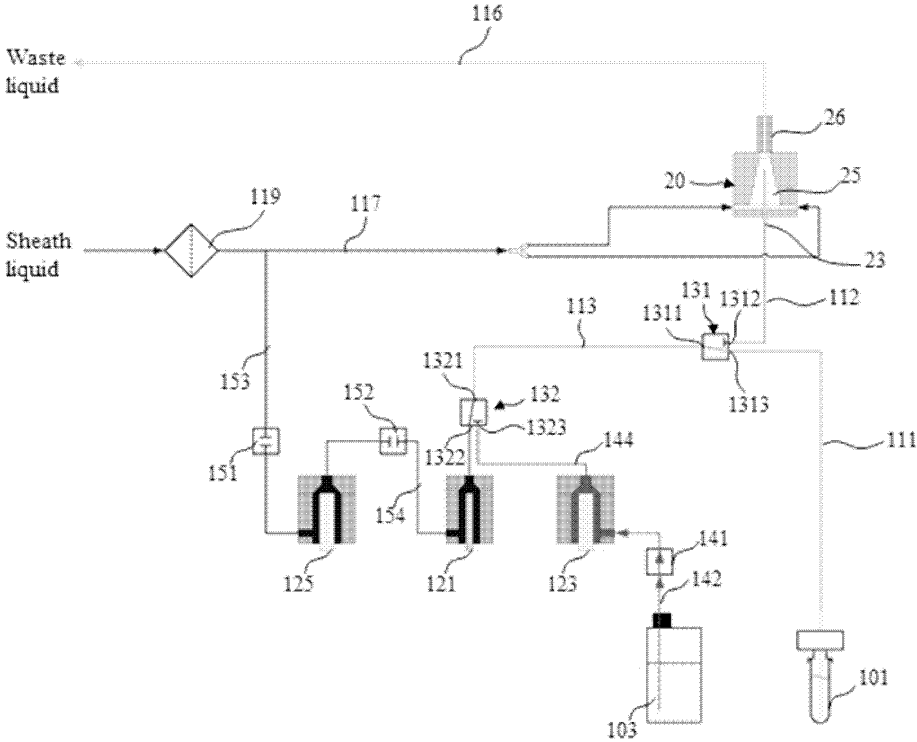


FIG.4

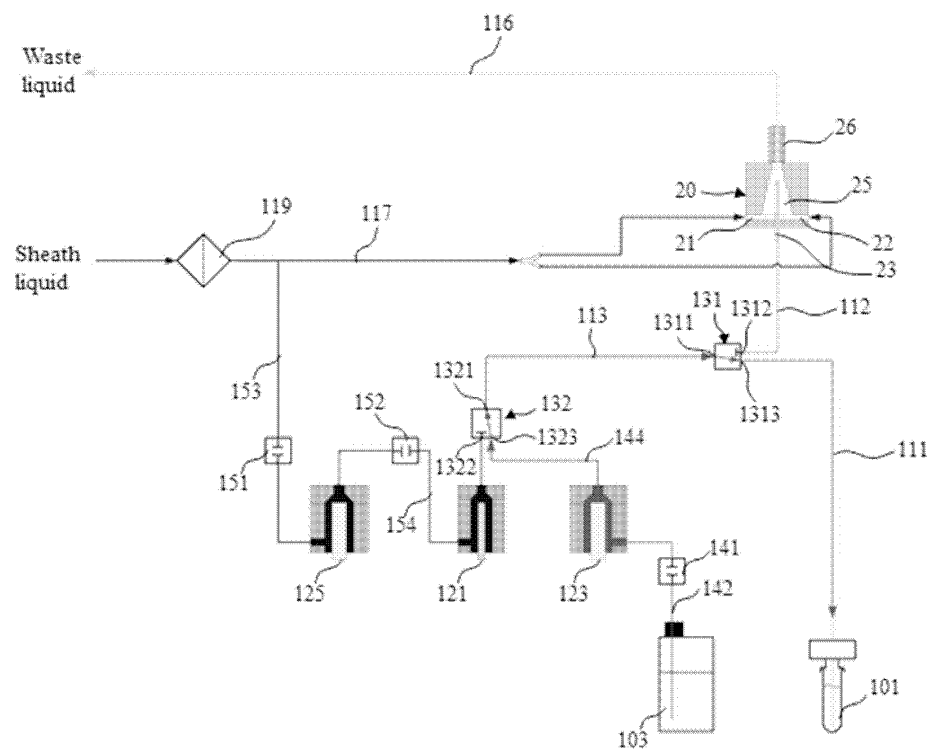


FIG.5

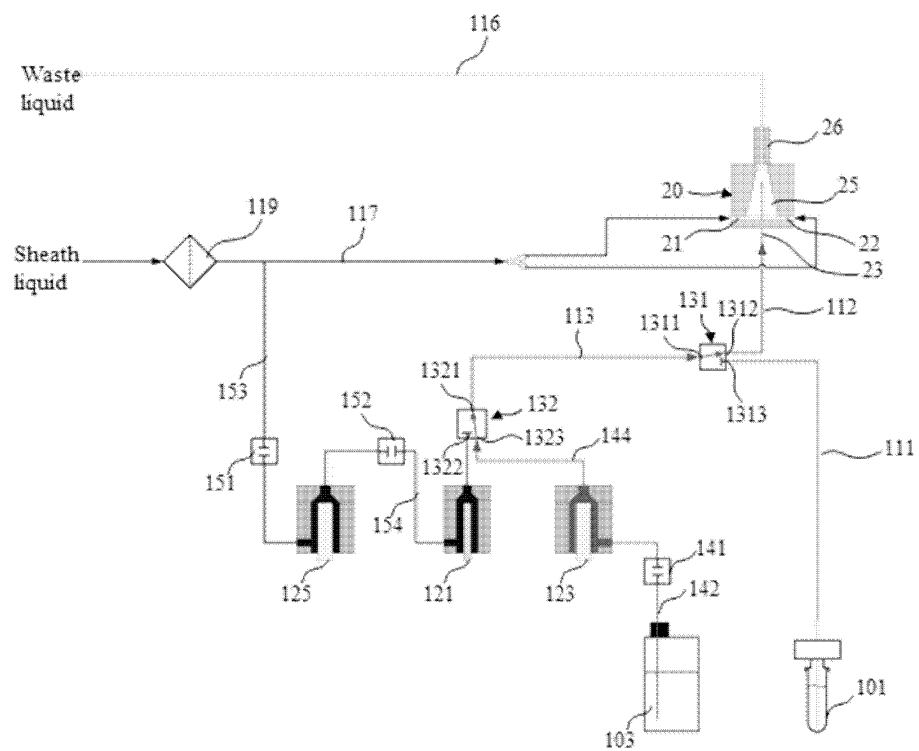


FIG.6

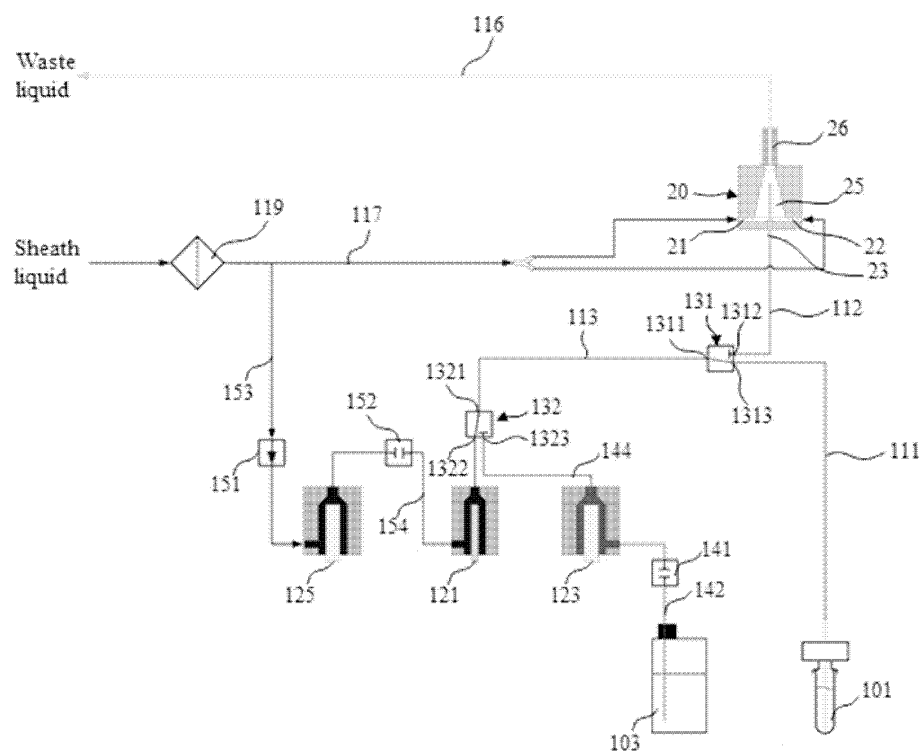


FIG. 7

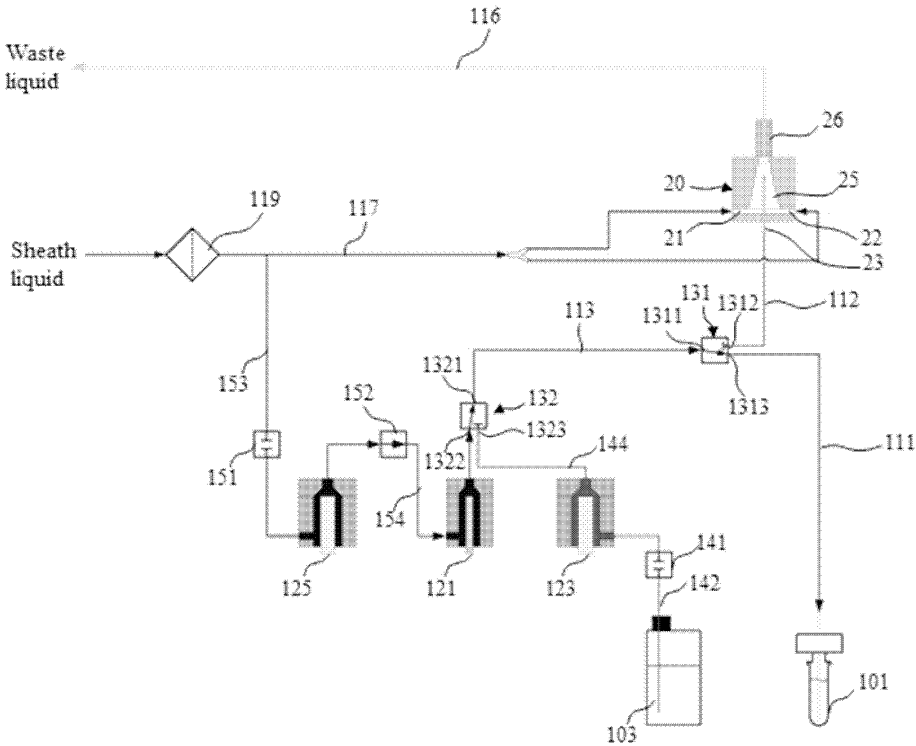


FIG.8

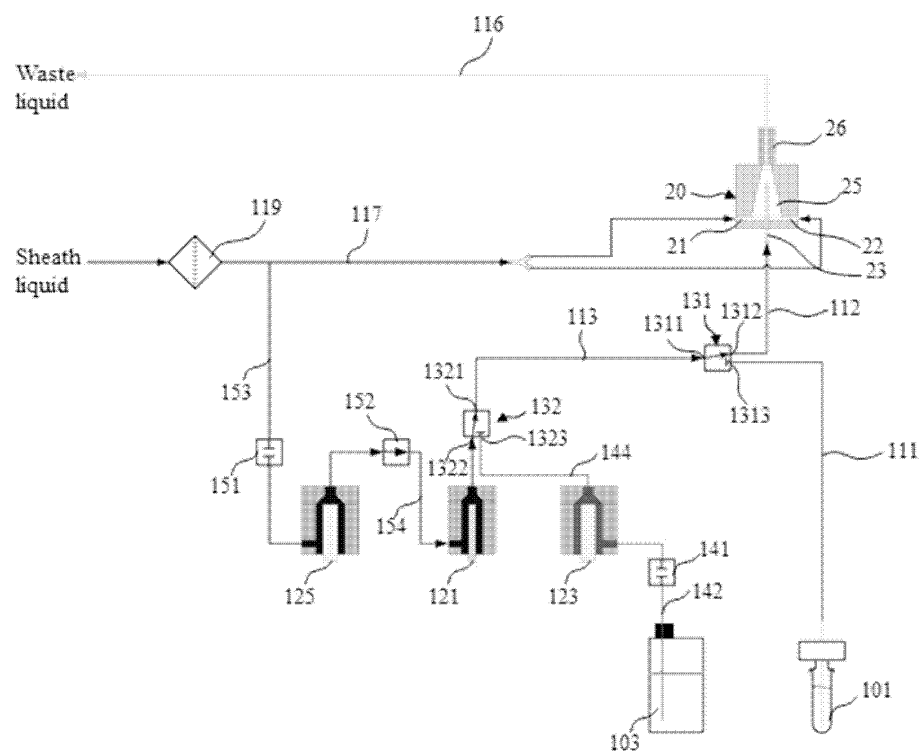


FIG.9

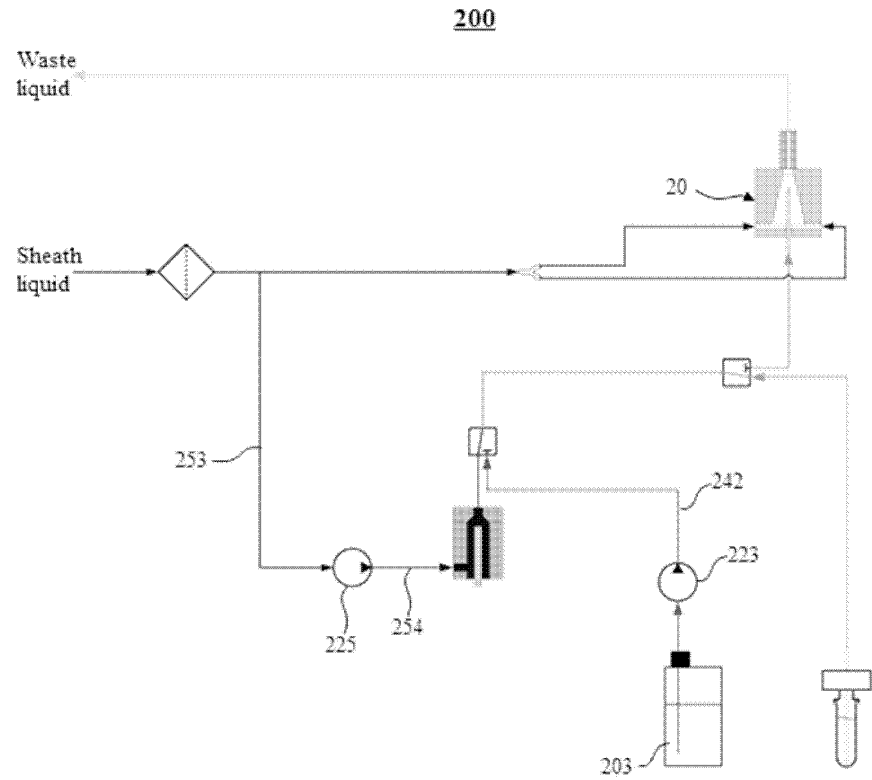


FIG.10

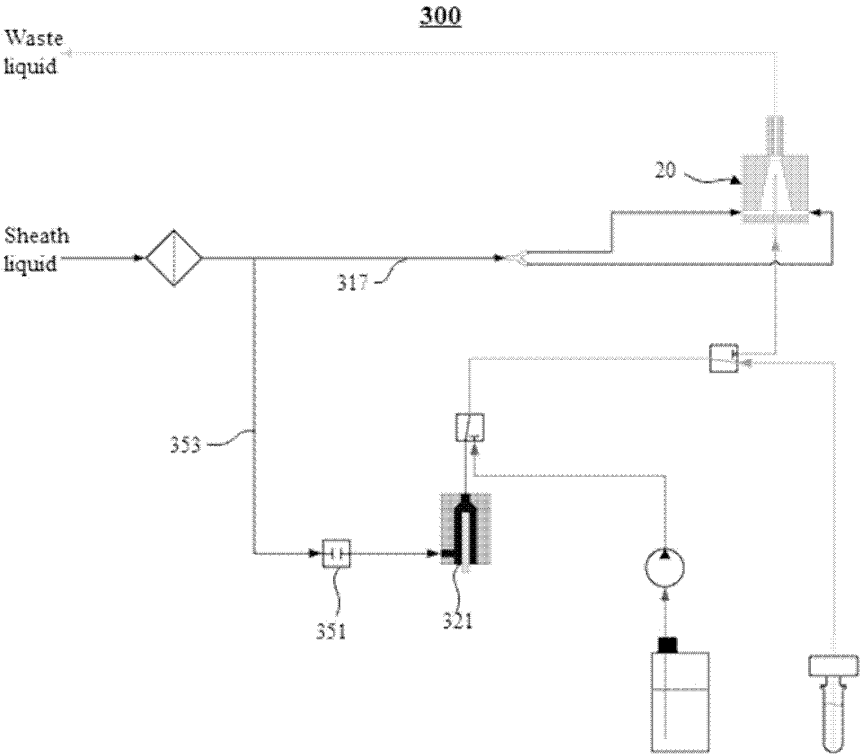


FIG.11

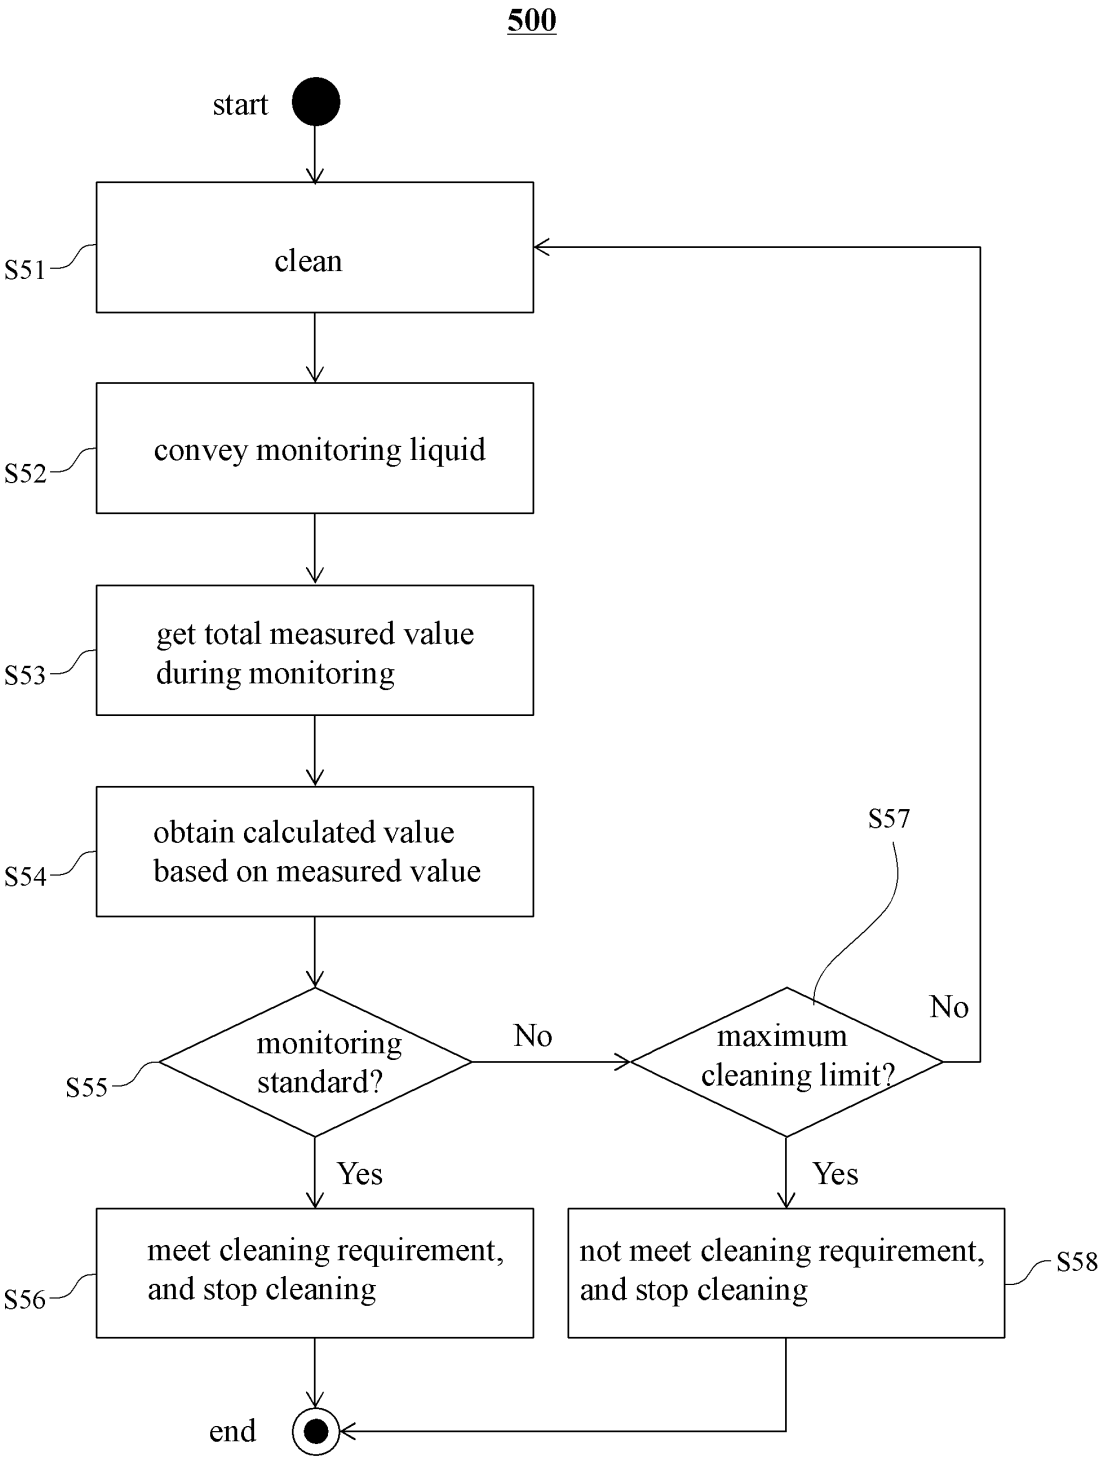


FIG.12

600

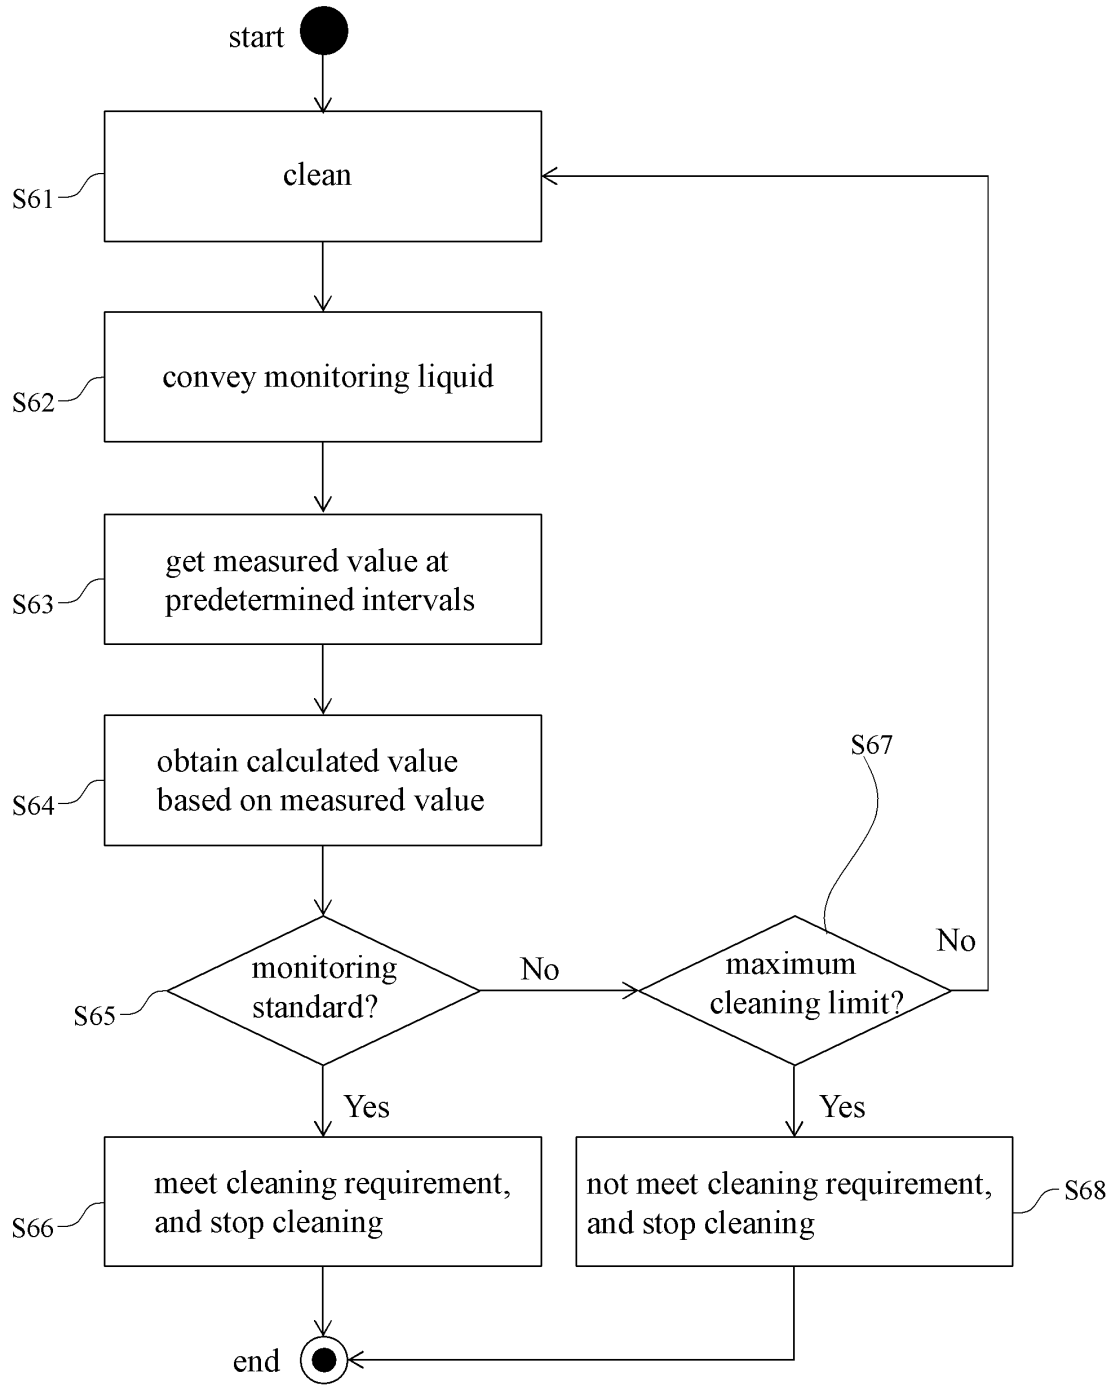


FIG.13

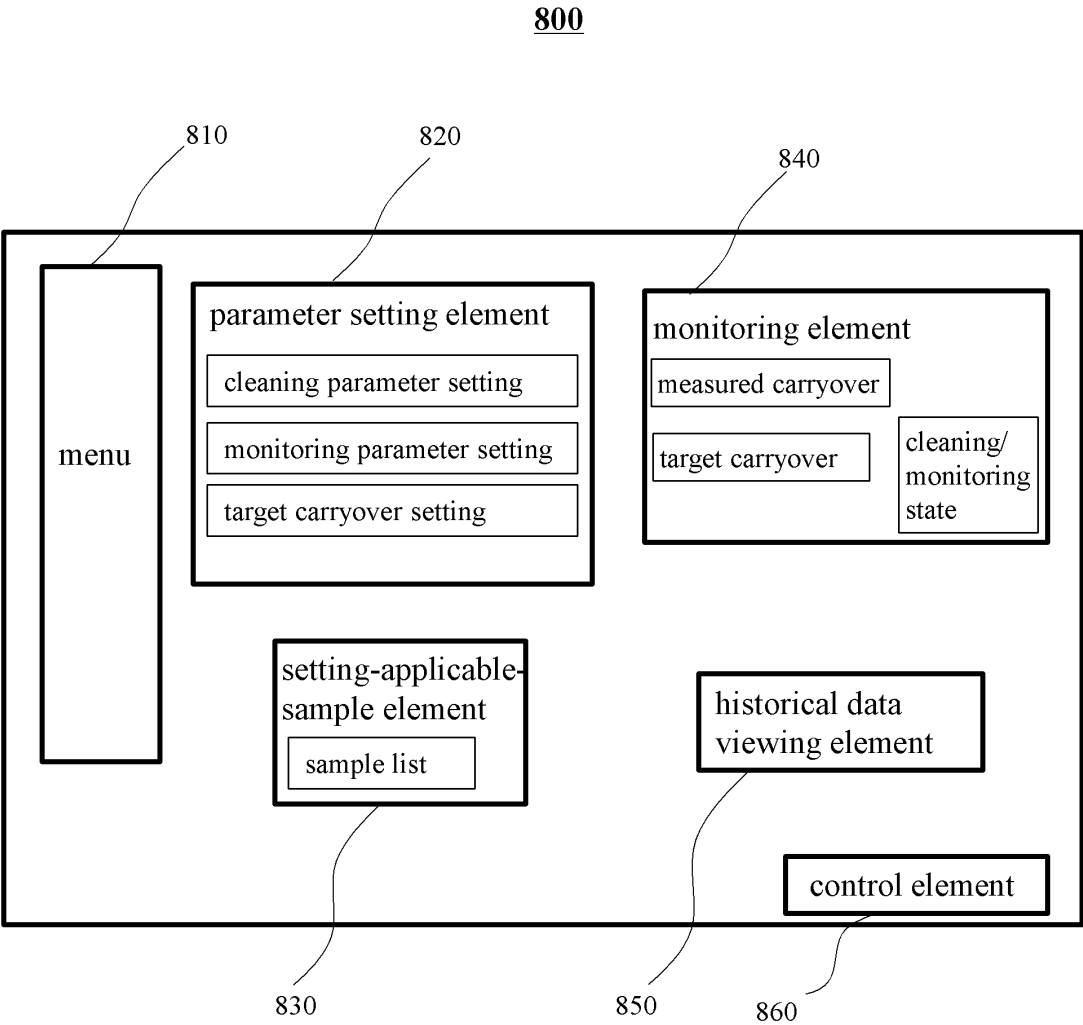


FIG.14

810

Sample

	Sample Name	Sample ID
☐	Sample 1	

Parameter Setting

Setting Applicable Samples

Operating Cleaning/Monitoring

View Monitoring Report

FIG.15

820

Parameter Setting

Cleaning/Monitoring

Cleaning Time:

1

min

Monitoring Solution Delivery Time:

3

min

Maximum Cleaning Cycles:

3

Cleaning Standard

Population:

P1

▼

☒ Carryover Rate (Events/Sec)

<=

10

☒ Concentration (Events/ μ L)

<=

600

☒ Cleaning and monitoring after processing the sample

Apply

Cancel

FIG.16

830

Setting Applicable Samples

Sample Name

☒ Sample1

☒ Sample2

☐ Sample3

☐ All

Confirm

Cancel

FIG.17

841

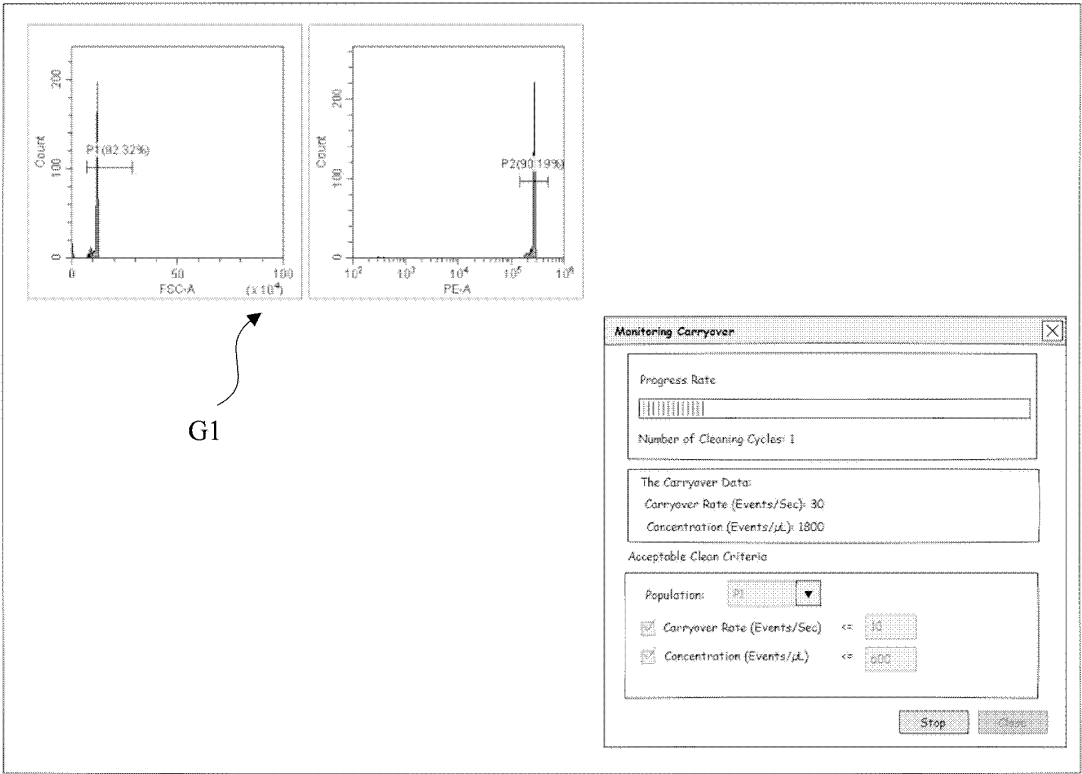


FIG.18A

842

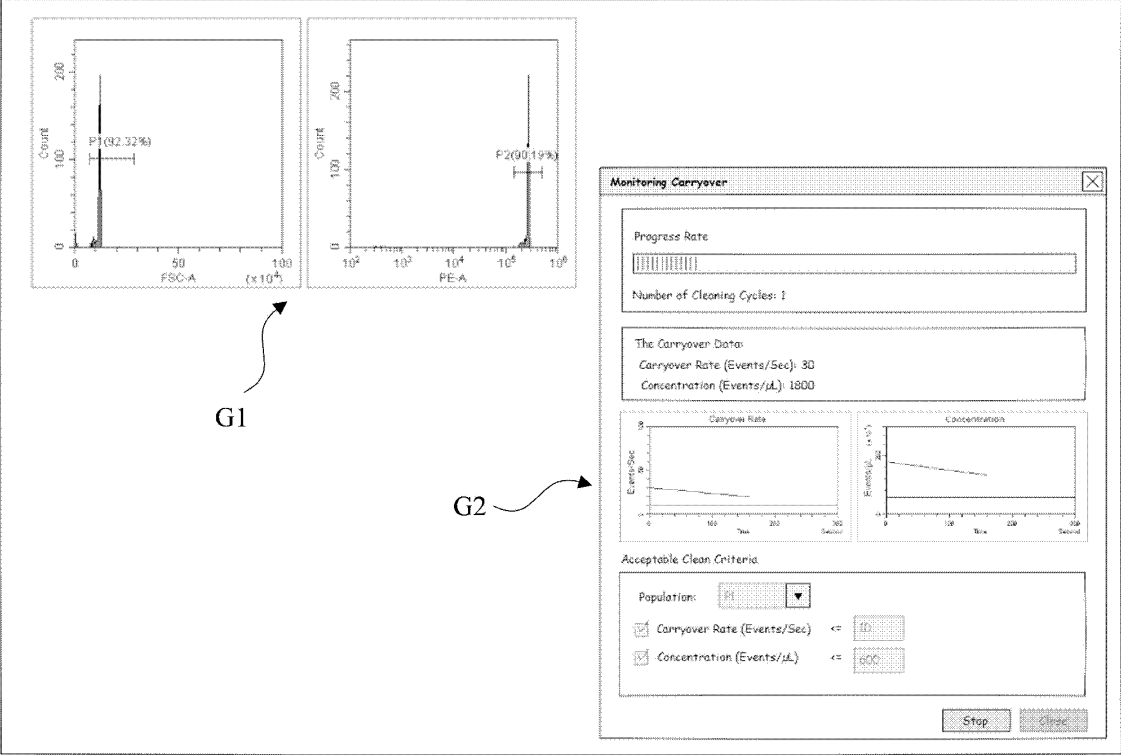


FIG.18B

843

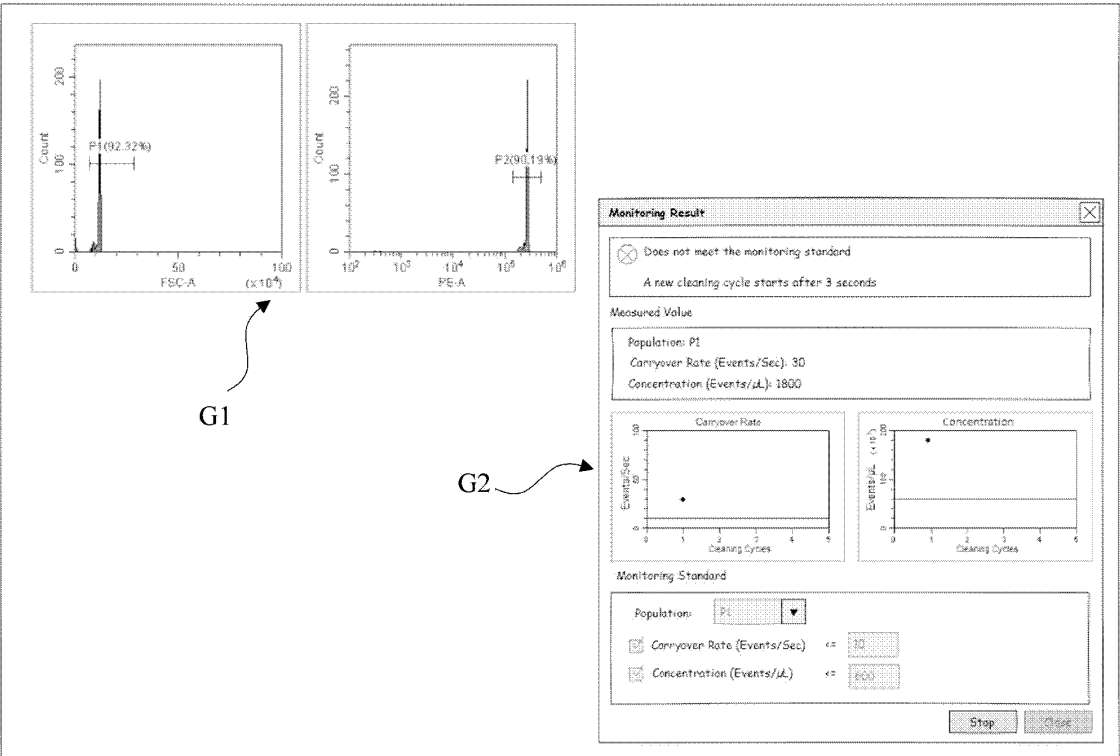


FIG.18C

844

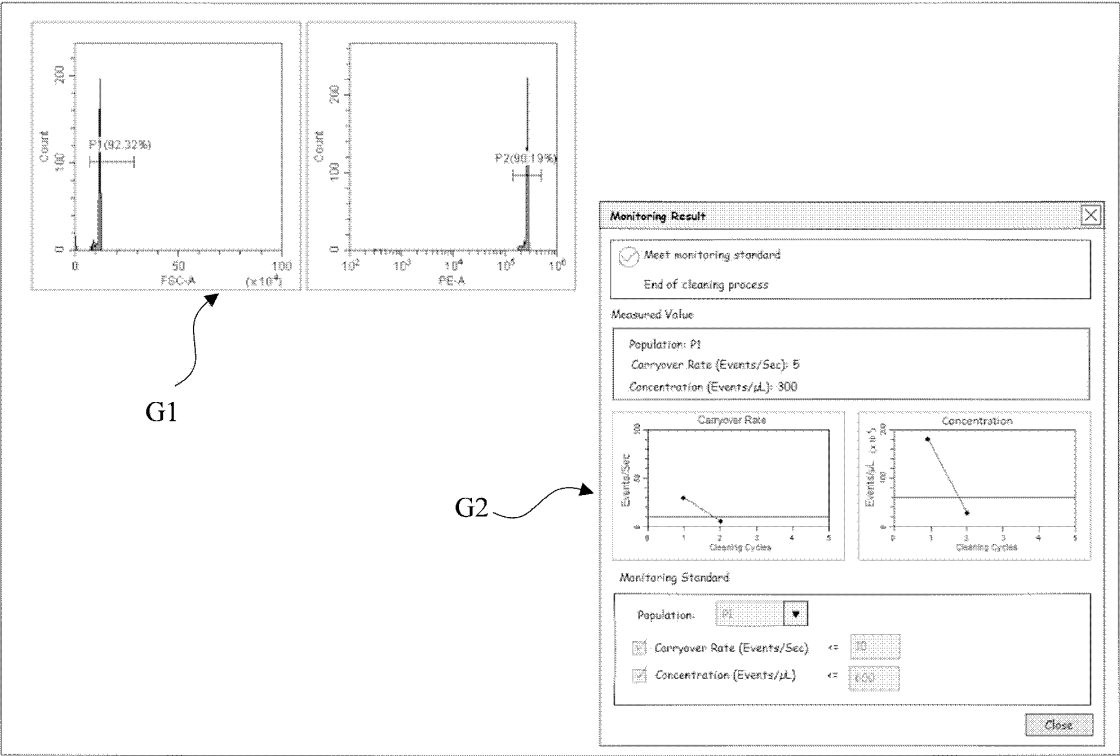


FIG.18D

845

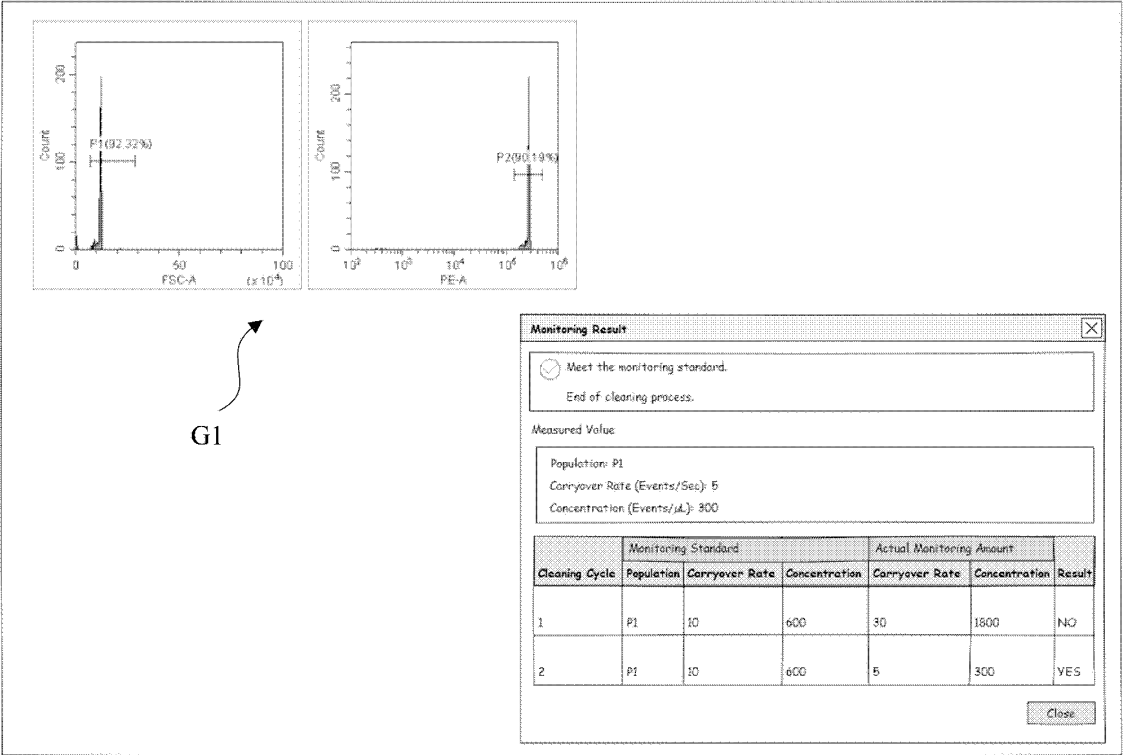


FIG.18E

850

Historical Monitoring Report								
Date	Sample	Monitoring Standard			Cleaning Cycle	Actual Monitoring Amount		Result
		Population	Carryover Rate (Events/Sec)	Concentration (Events/ μ L)		Carryover Rate (Events/Sec)	Concentration (Events/ μ L)	
2021-1-01 10:00	Sample1	P1	10	600	3	20	1200	NO
2021-1-01 10:20	Sample2	P1	10	600	1	5	300	YES
2021-1-01 10:30	Sample3	P1	10	600	1	5	300	YES
ExportConfirmCancel								

FIG.19

900

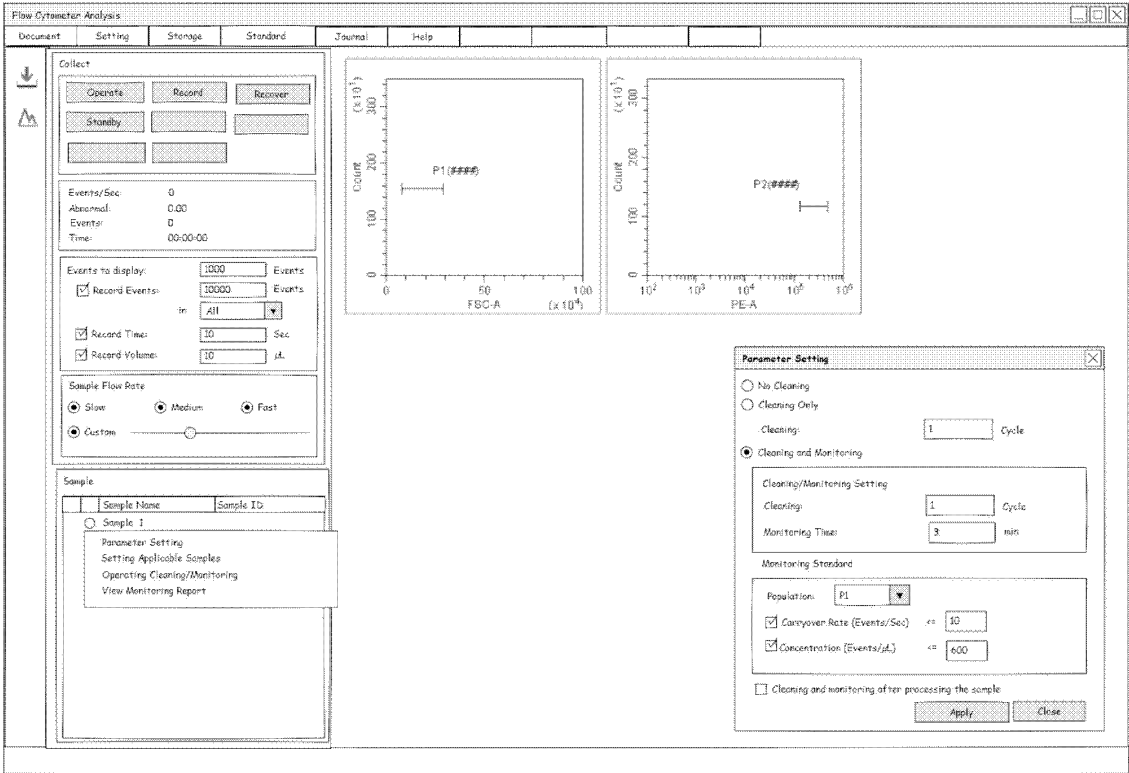


FIG.20