

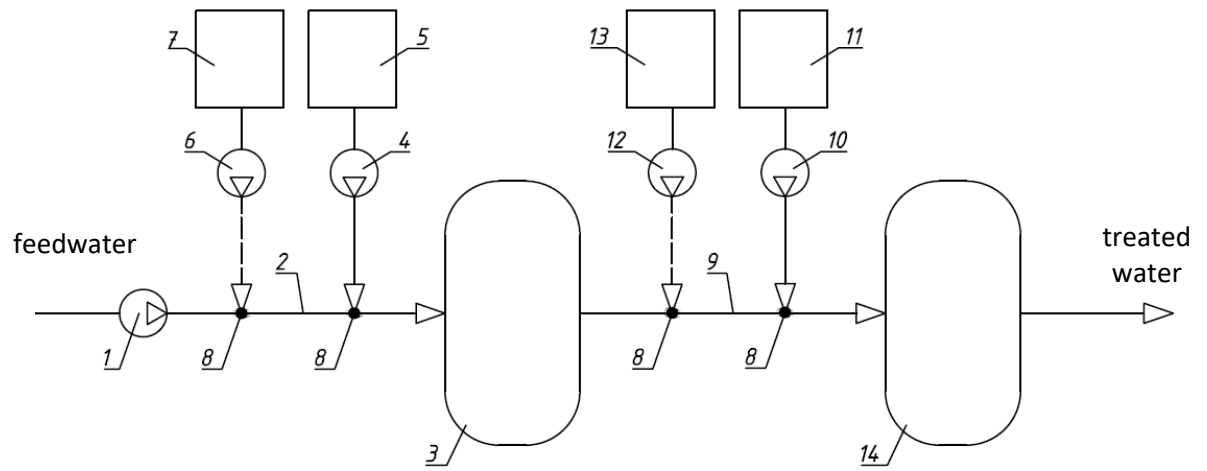


Fig. 1

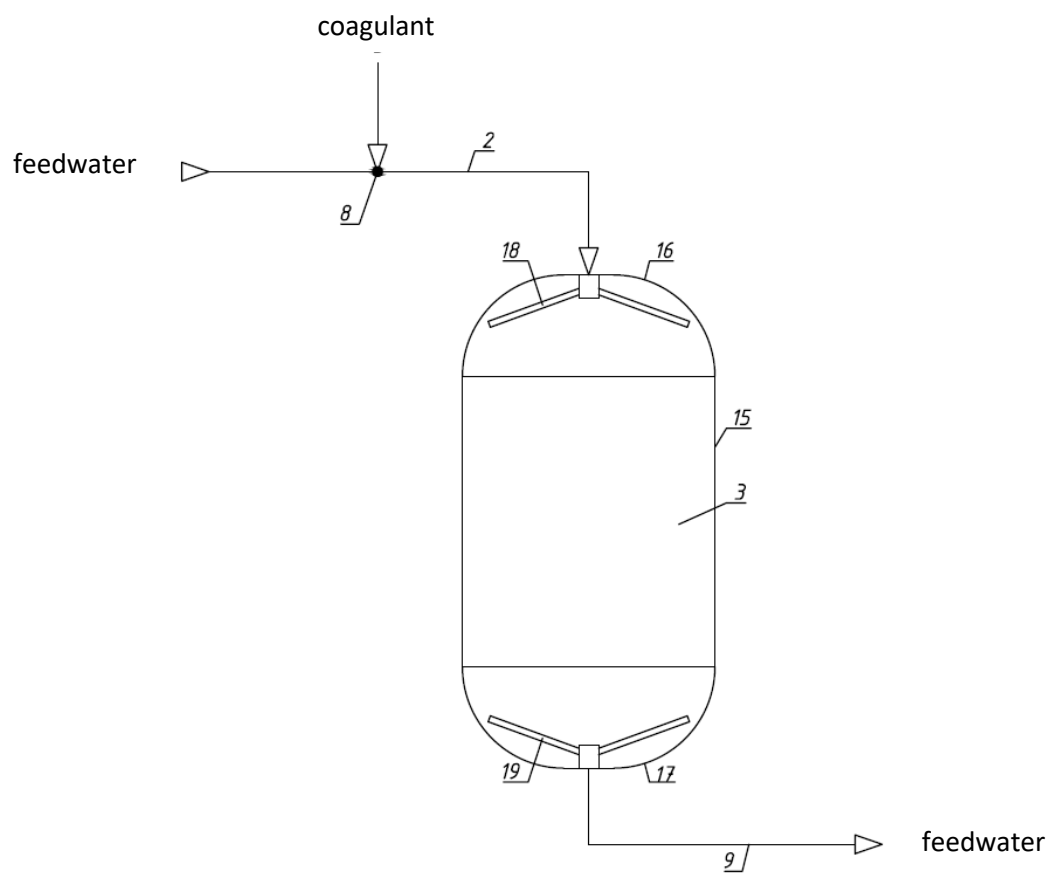


Fig. 2

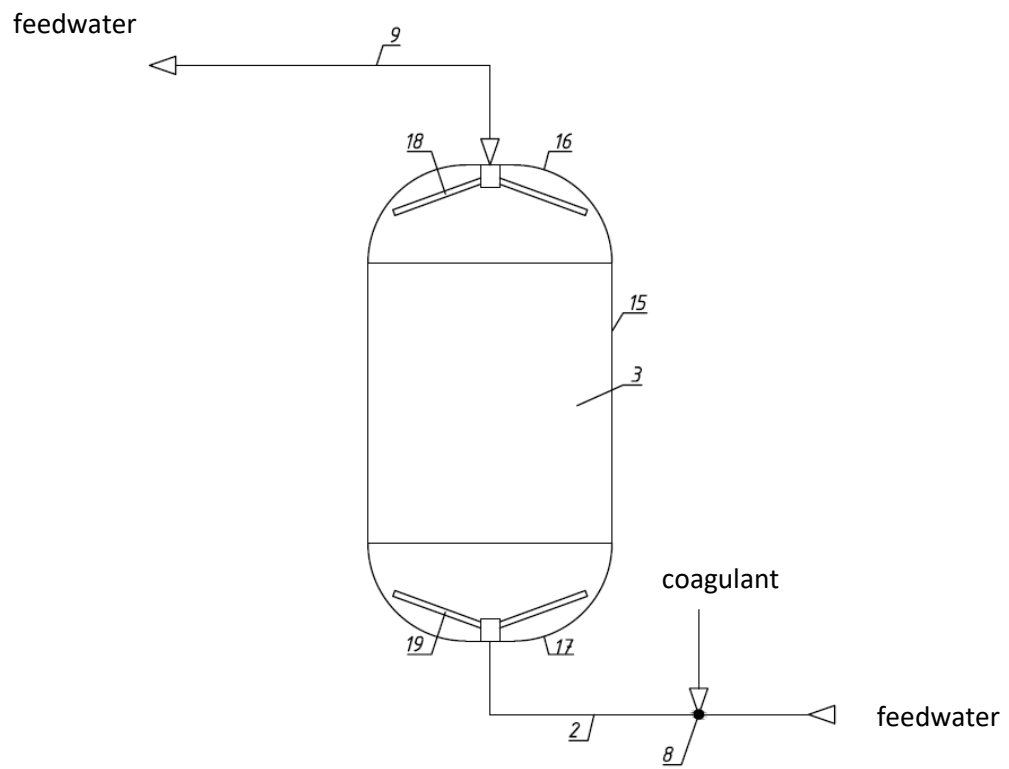


Fig. 3

removal of
contaminant light
fractions

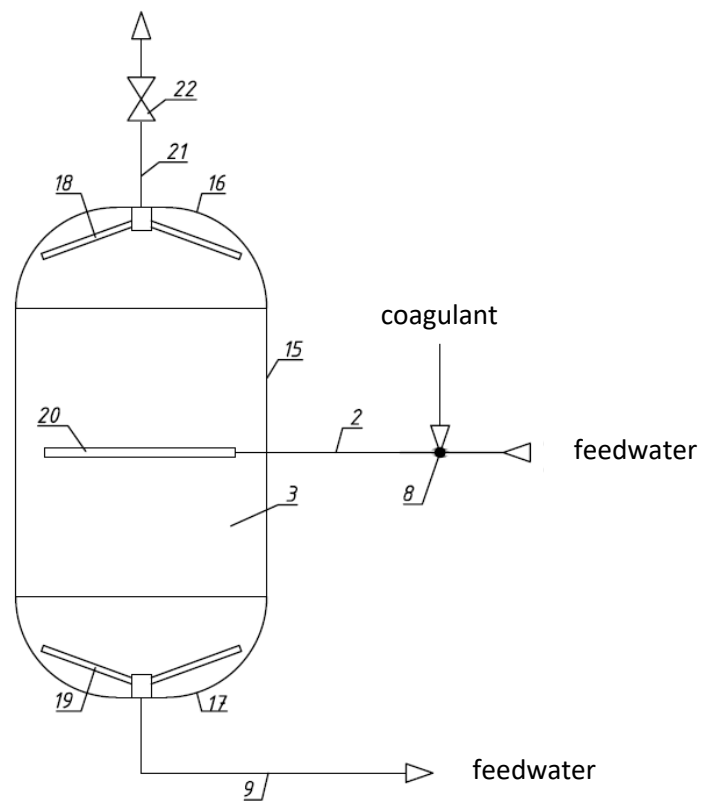


Fig. 4

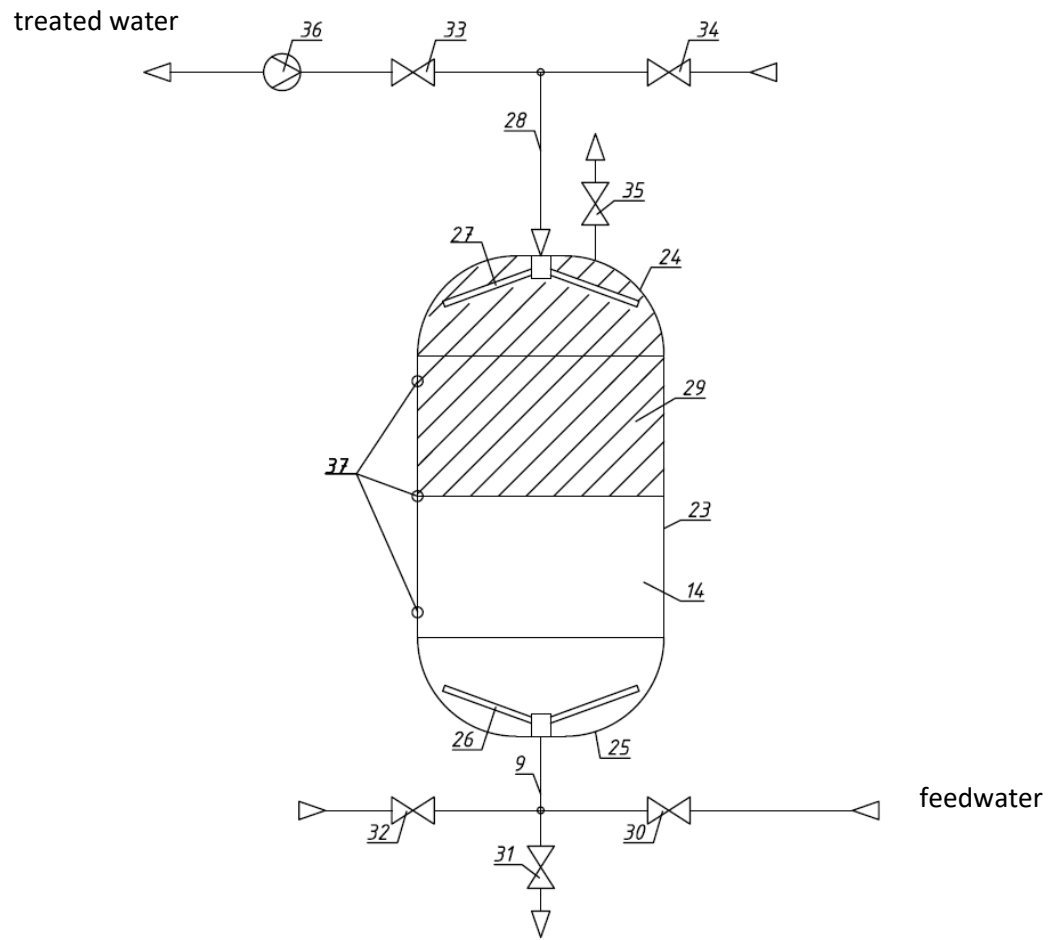


Fig. 5

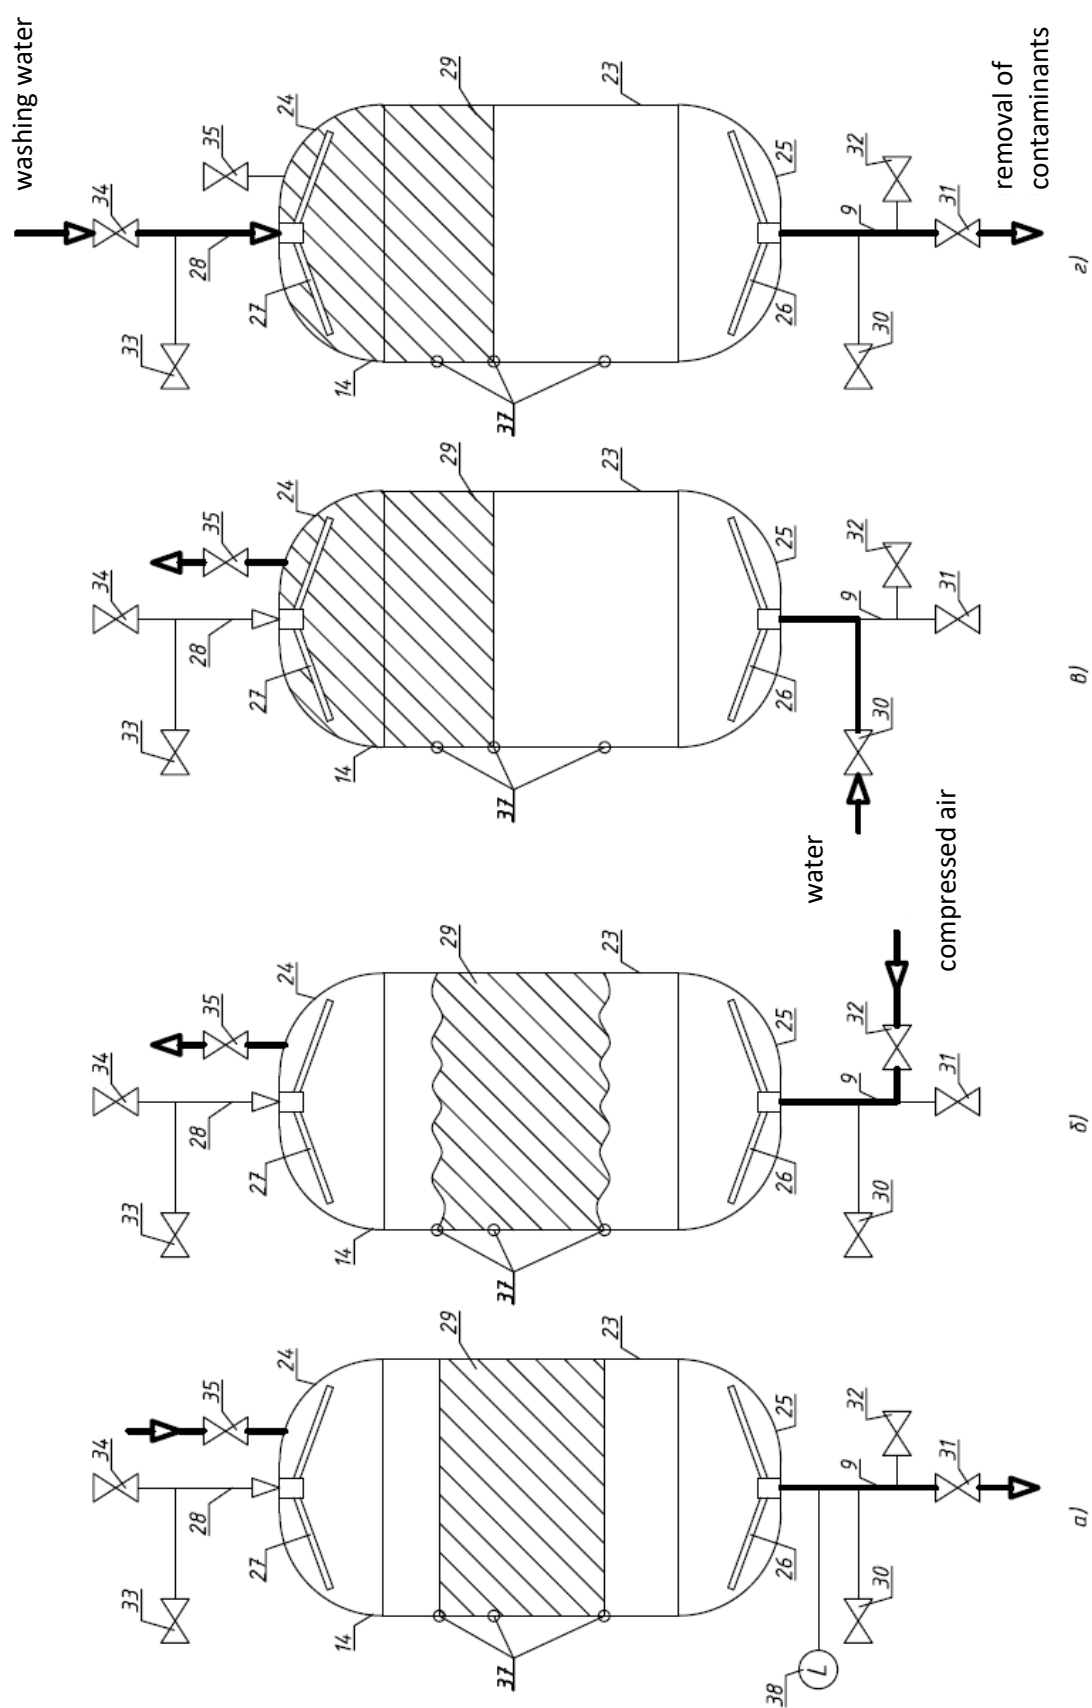


Fig. 6

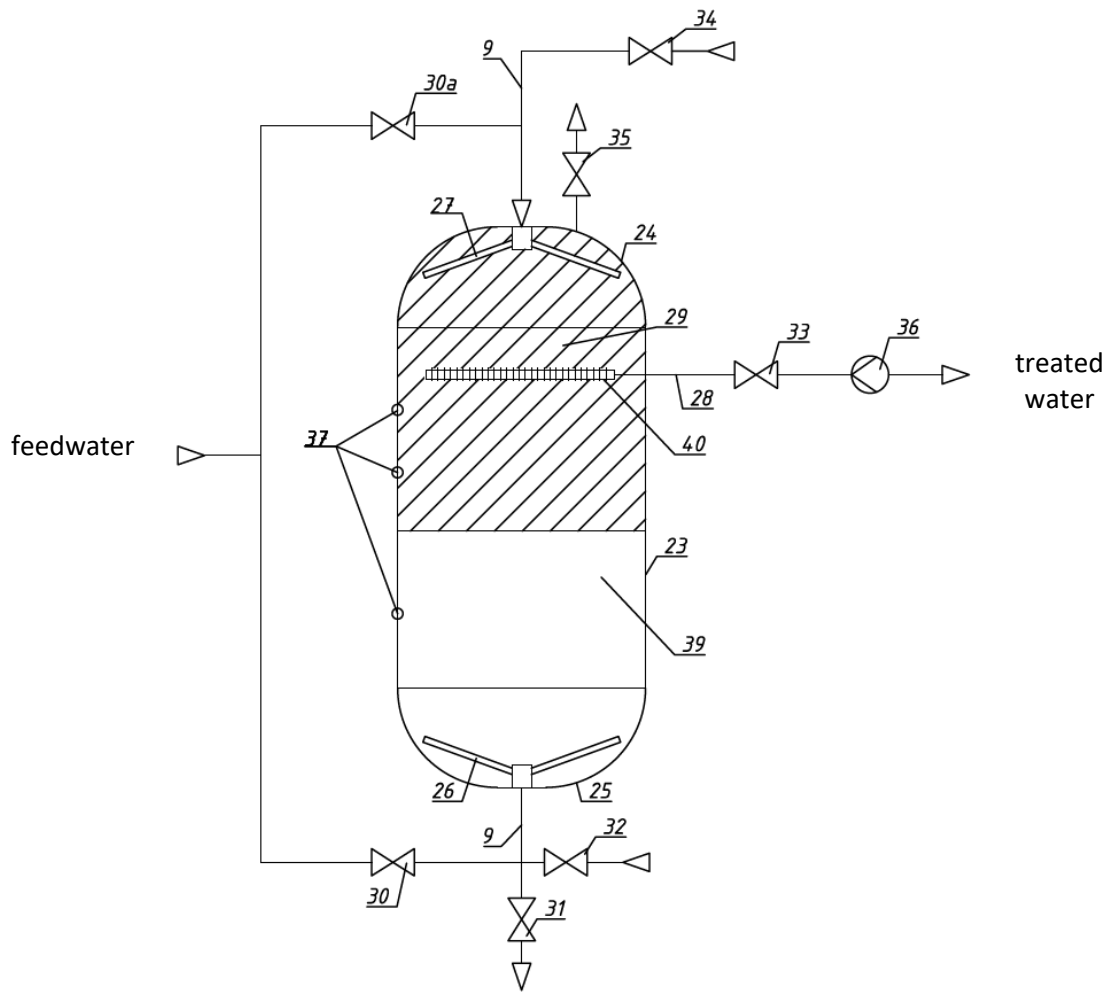


Fig. 7


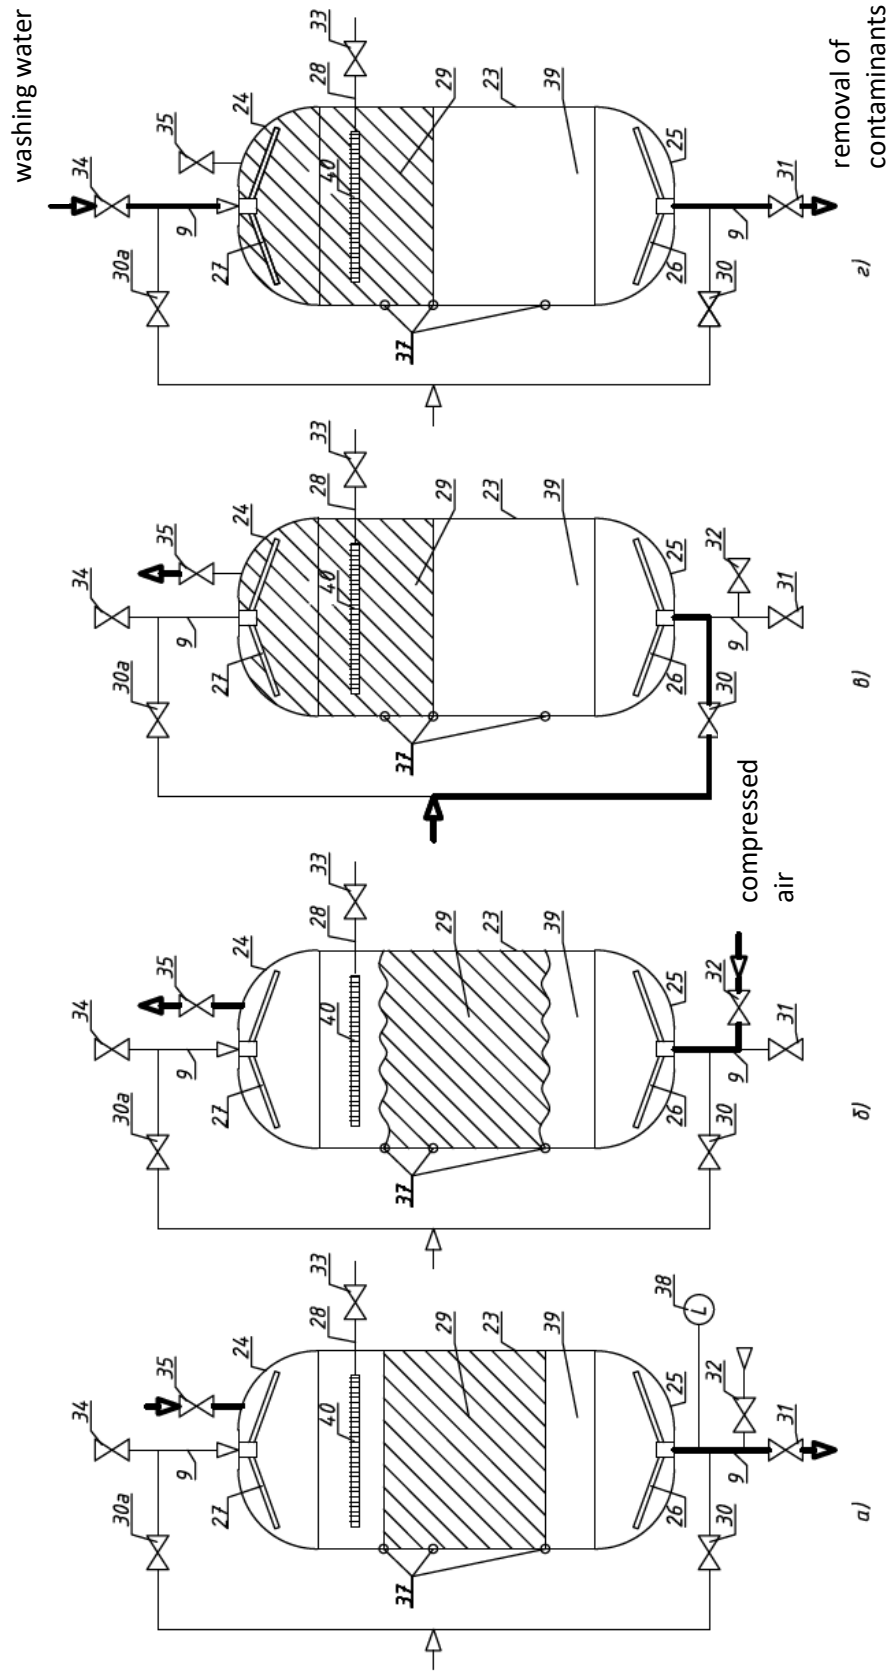


Fig. 8

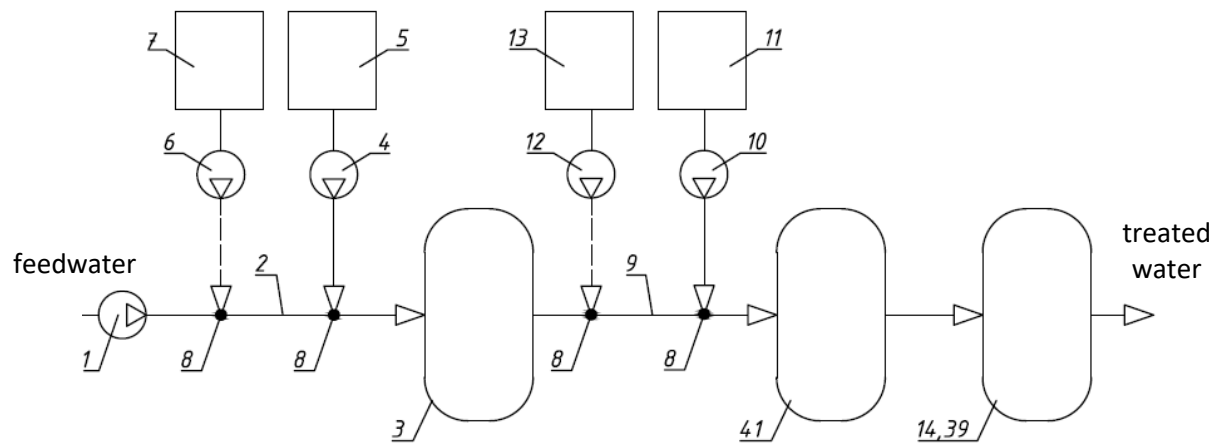

Фиг. 9

Fig. 9

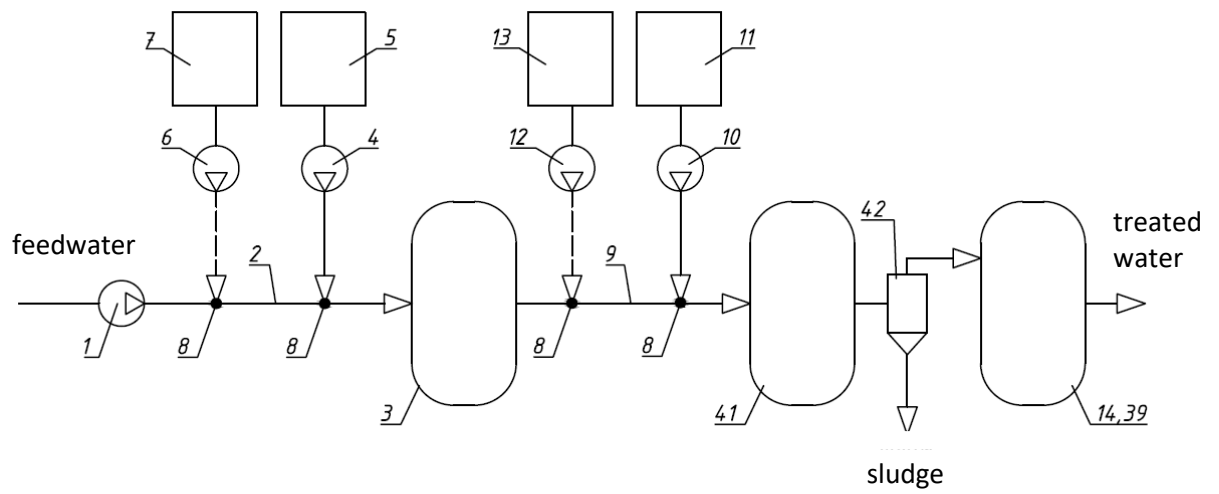


Fig. 10