

FIG. 1



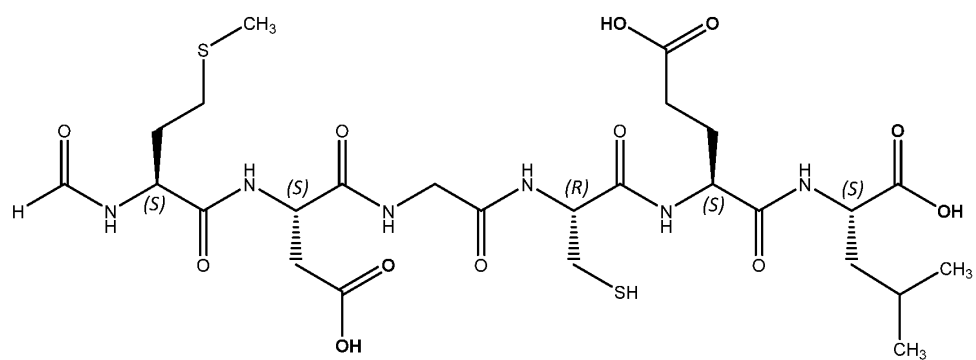


FIG. 2

A)

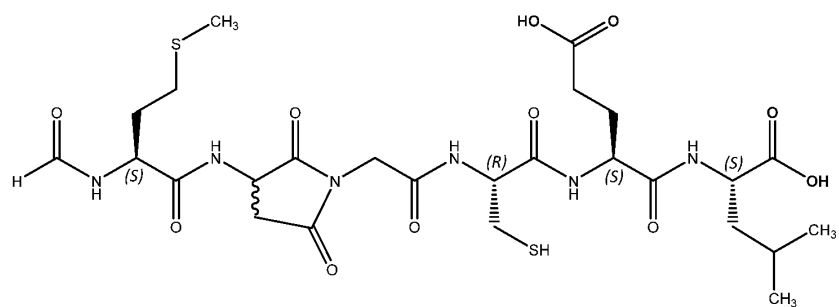

B)

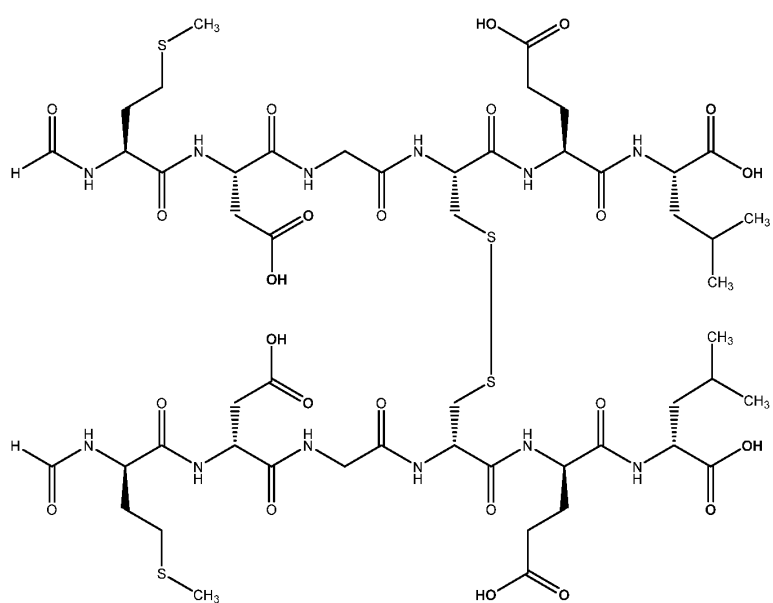

C)

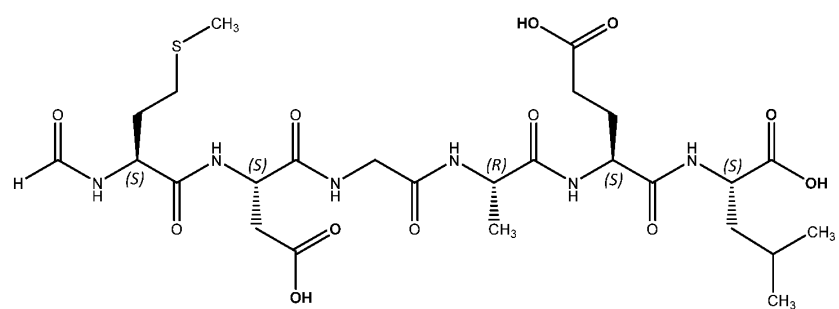


FIG. 3

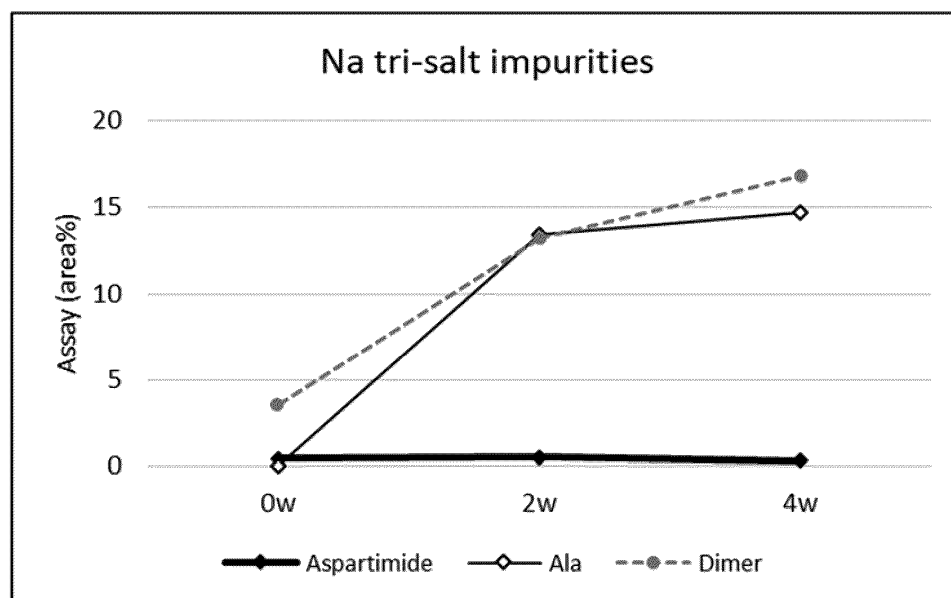


FIG.4

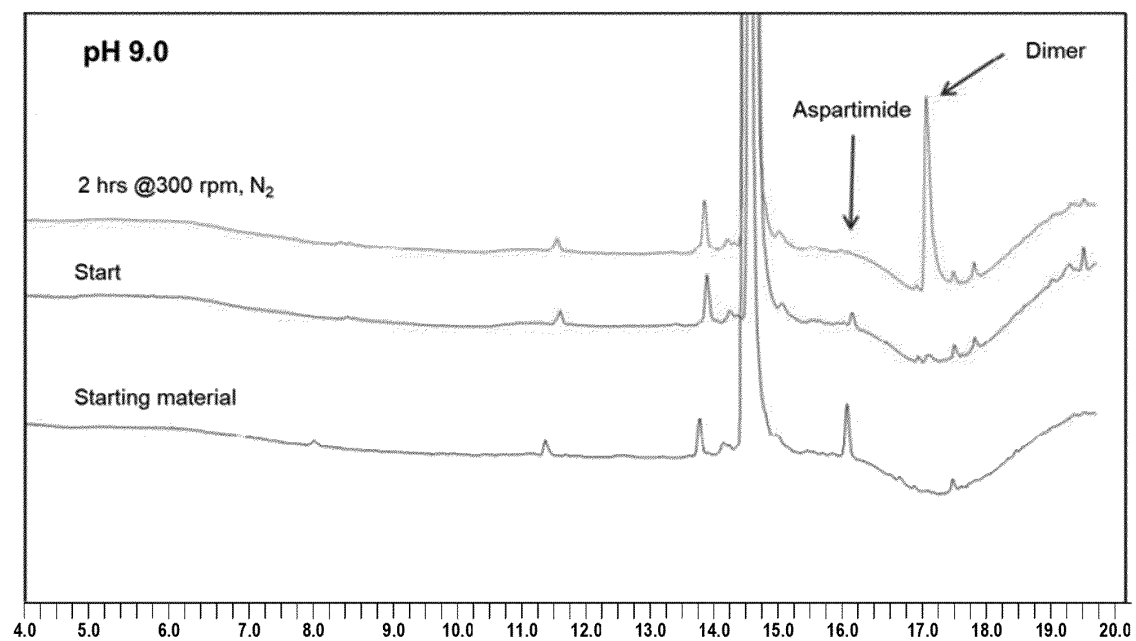


FIG. 5

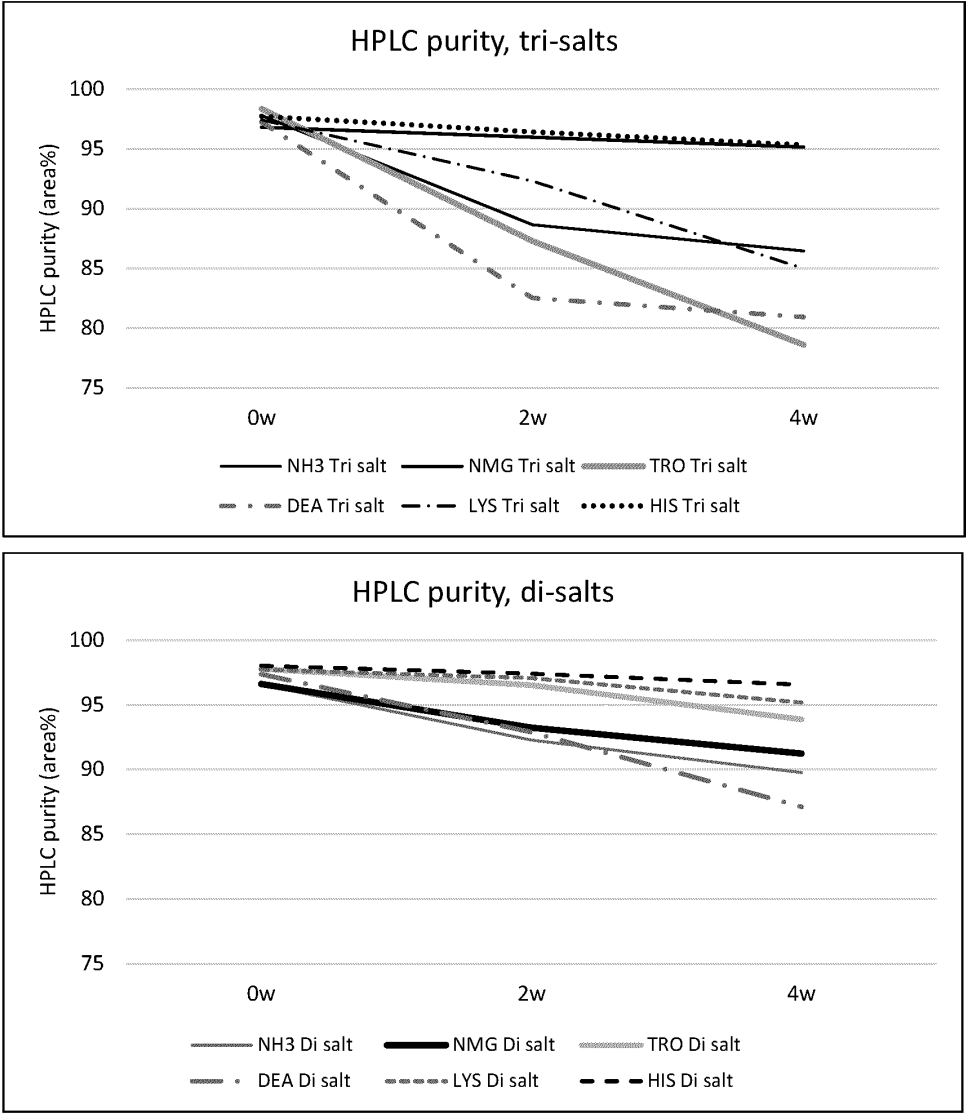


FIG. 6

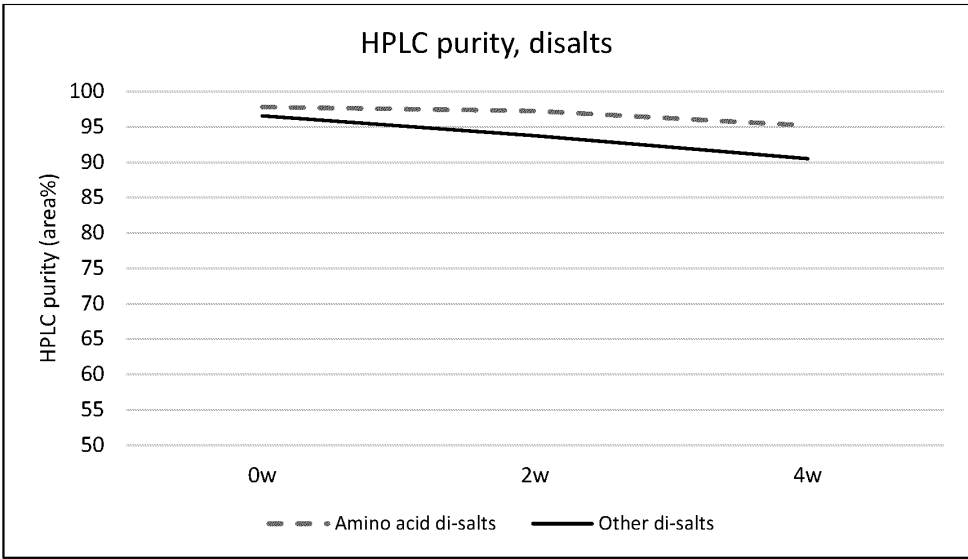
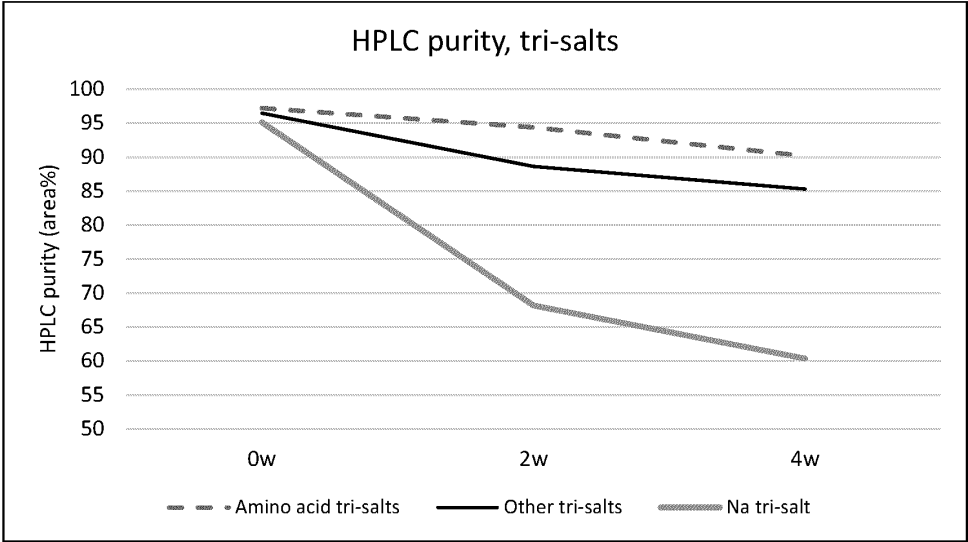


FIG. 7

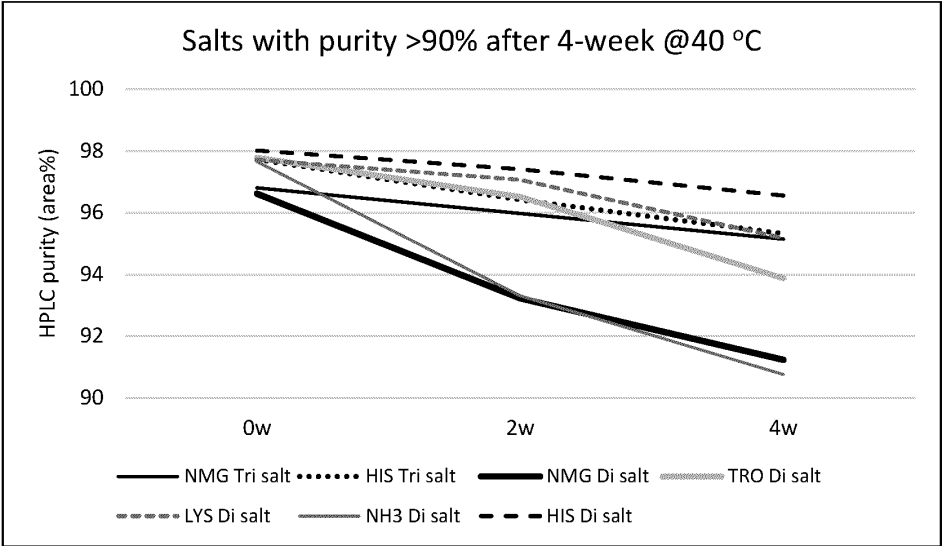


FIG. 8

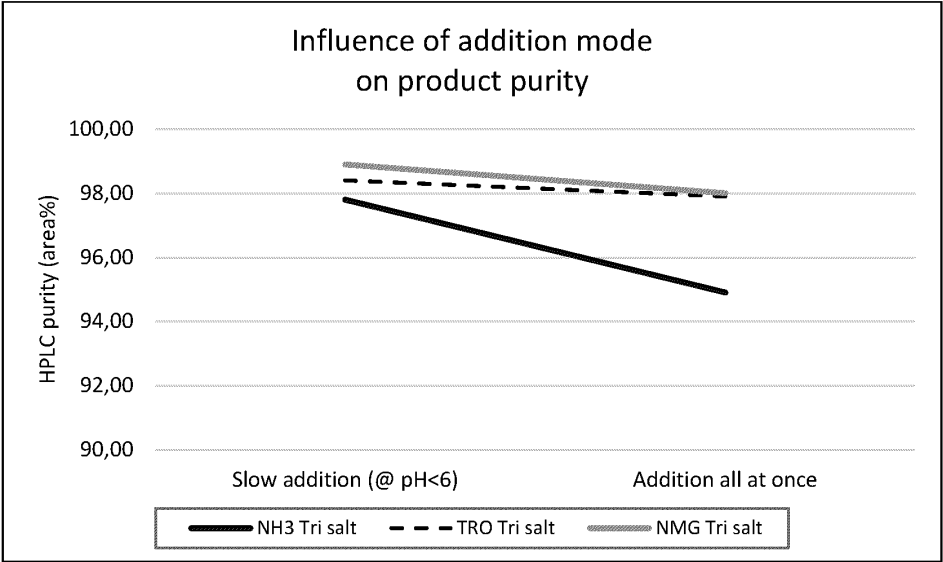


FIG. 9

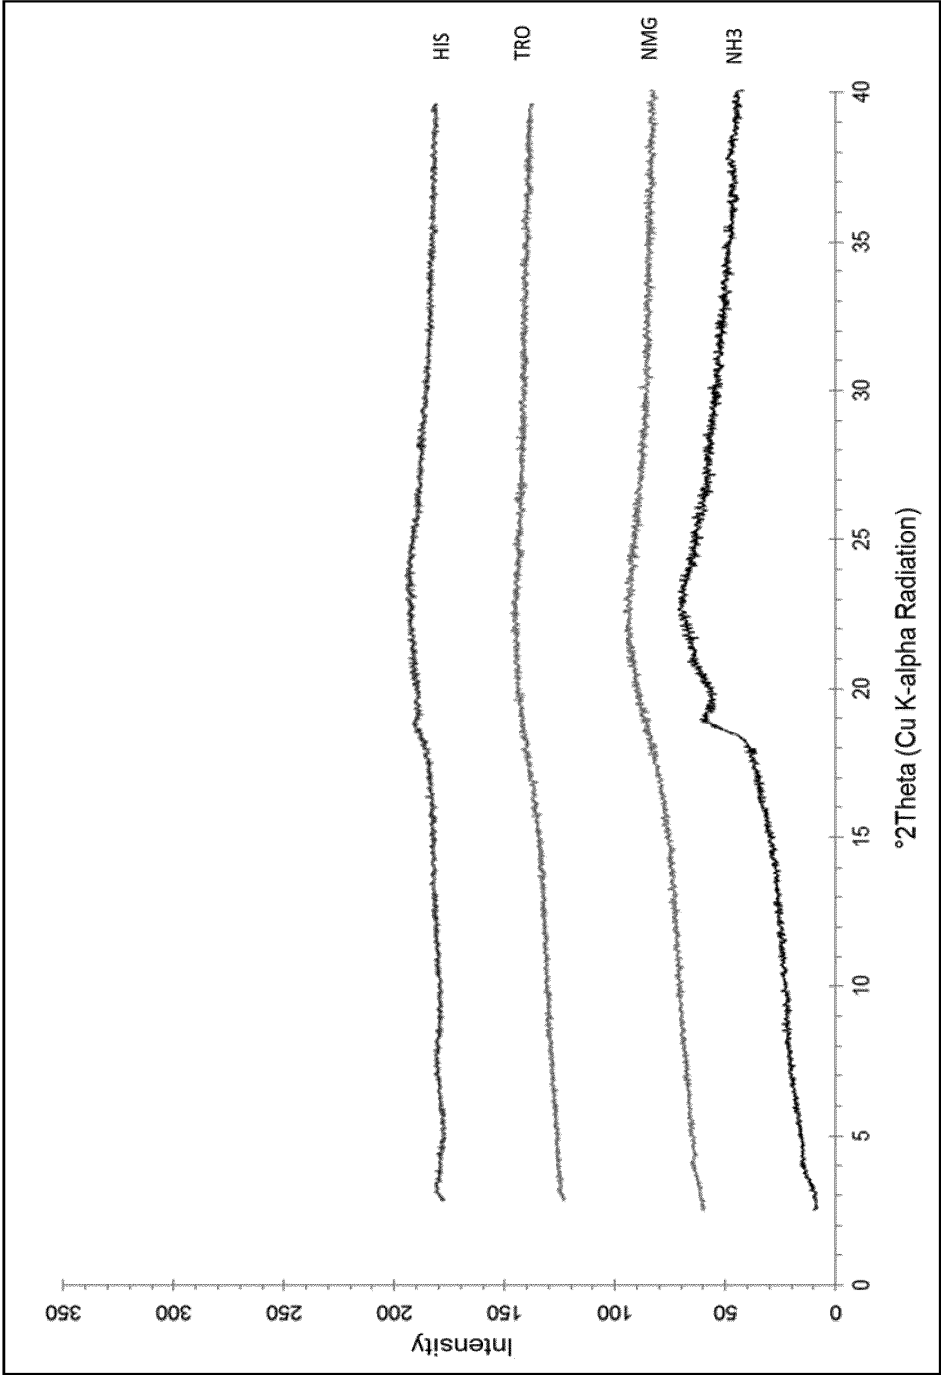


FIG. 10

Compound	Initial				After 2 weeks @ 40°C				After 4 weeks @ 40°C			
	HPLC purity (area%)	Ala (area%)	Aspartimide (area%)	Dimer (area%)	HPLC purity (area%)	Ala (area%)	Aspartimide (area%)	Dimer (area%)	HPLC purity (area%)	Ala (area%)	Aspartimide (area%)	Dimer (area%)
Foxy-5 free acid	98.40	0.00	0.70	0.00	98.40	0	0.75	0.00	98.21	0.00	0.80	0.00
NH3 Tri salt	97.78	0.00	1.25	0.18	88.64	0	4.10	2.95	86.45	0.00	3.88	3.37
NMG Tri salt	96.80	0.00	2.08	0.38	95.97	0	1.76	1.13	95.14	0.00	3.06	0.82
TRO Tri salt	98.35	0.00	0.97	0.00	87.27	0	8.24	0.63	78.60	0.00	11.40	1.28
DEA Tri salt	97.24	0.00	0.67	0.00	82.51	1.91	5.78	8.10	80.92	1.82	7.20	5.80
LYS Tri salt	97.42	0.25	0.55	0.48	92.29	4.25	1.10	1.80	84.97	8.45	1.26	3.40
ARG Tri salt	96.44	0.30	0.41	1.30	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A
CHO Tri salt	92.11	0.71	0.00	5.12	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A
HIS Tri salt	97.72	0.00	1.18	0.45	96.41	0	1.97	1.10	95.32	0.00	2.43	0.90
Na Tri salt	95.11	0.00	0.45	3.49	68.15	13.4	0.53	13.20	60.34	14.70	0.30	16.80
NH3 Di salt	96.57	0.00	2.10	0.22	92.27	0	4.45	0.38	89.75	0.00	5.52	0.27
NMG Di salt	96.61	0.00	2.27	0.35	93.22	0	3.85	0.93	91.23	0.00	6.17	0.81
TRO Di salt	97.78	0.00	0.93	0.00	96.51	0	2.75	0.00	93.87	0.00	4.20	0.60
DEA Di salt	97.36	0.00	0.90	0.00	92.88	0	4.98	1.18	87.11	0.25	7.50	3.10
LYS Di salt	97.71	0.00	0.97	0.00	97.06	0	2.50	0.00	95.17	0.47	2.80	0.55
HIS Di salt	98.01	0.00	1.37	0.00	97.40	0	1.97	0.00	96.52	0.00	2.40	0.00
ARG Di salt	97.69	0.00	0.97	0.00	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A
CHO Di salt	94.35	0.52	0.80	1.18	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A

FIG. 11

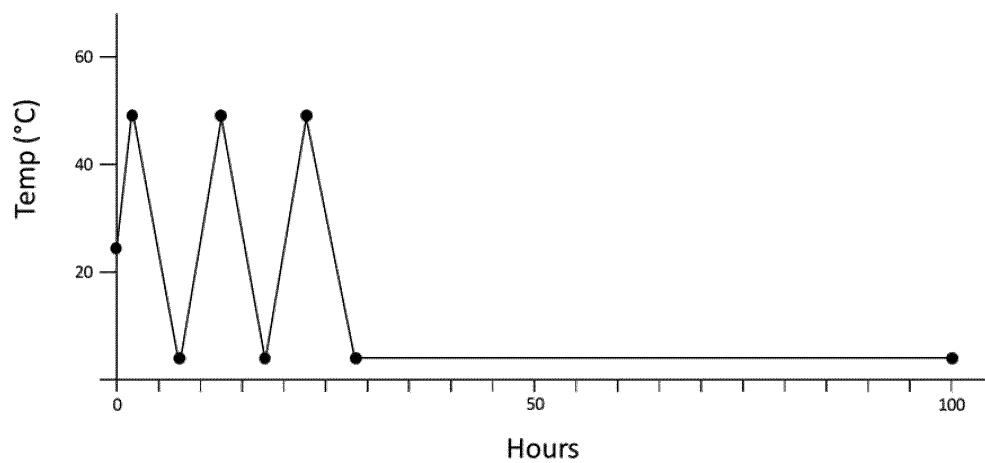


FIG. 12

Sample	Foxy-5	L-His	Calibration line	Measured area	Theor. conc (mg/ml)	Measured conc (mg/ml)	Ratio
HIS-GEN2	1	1	50.6700	43.7400	0.0947	0.0870	0.92
GEN5	1	2	50.6700	47.3520	0.0989	0.0942	1.90
GEN8	1	3	50.6700	47.9130	0.0995	0.0953	2.87
GEN14	1	2	43.6040	45.4890	0.0977	0.1023	2.10
HIS-GEN15	1	3	43.6040	46.2290	0.0978	0.1040	3.19
TCP7	1	2	43.6040	38.5390	0.0980	0.0867	1.77
TCP11	1	3	43.6040	41.1940	0.0962	0.0927	2.89

Sample	Foxy-5	NMG	Calibration line	Measured area	Theor. conc (mg/ml)	Measured conc (mg/ml)	Ratio
NMG-GEN4	1	1	61.2490	57.2330	0.0996	0.0959	0.96
GEN7	1	2	61.2490	59.4290	0.1000	0.0996	1.99
GEN10	1	3	61.2490	55.1580	0.0906	0.0924	3.06
NMG-GEN16	1	2	52.9390	43.7140	0.0771	0.0817	2.12
TCP18	1	2	52.9390	45.5720	0.0842	0.0852	2.03
TCP20	1	2	52.9390	47.9040	0.0876	0.0896	2.04

FIG.13

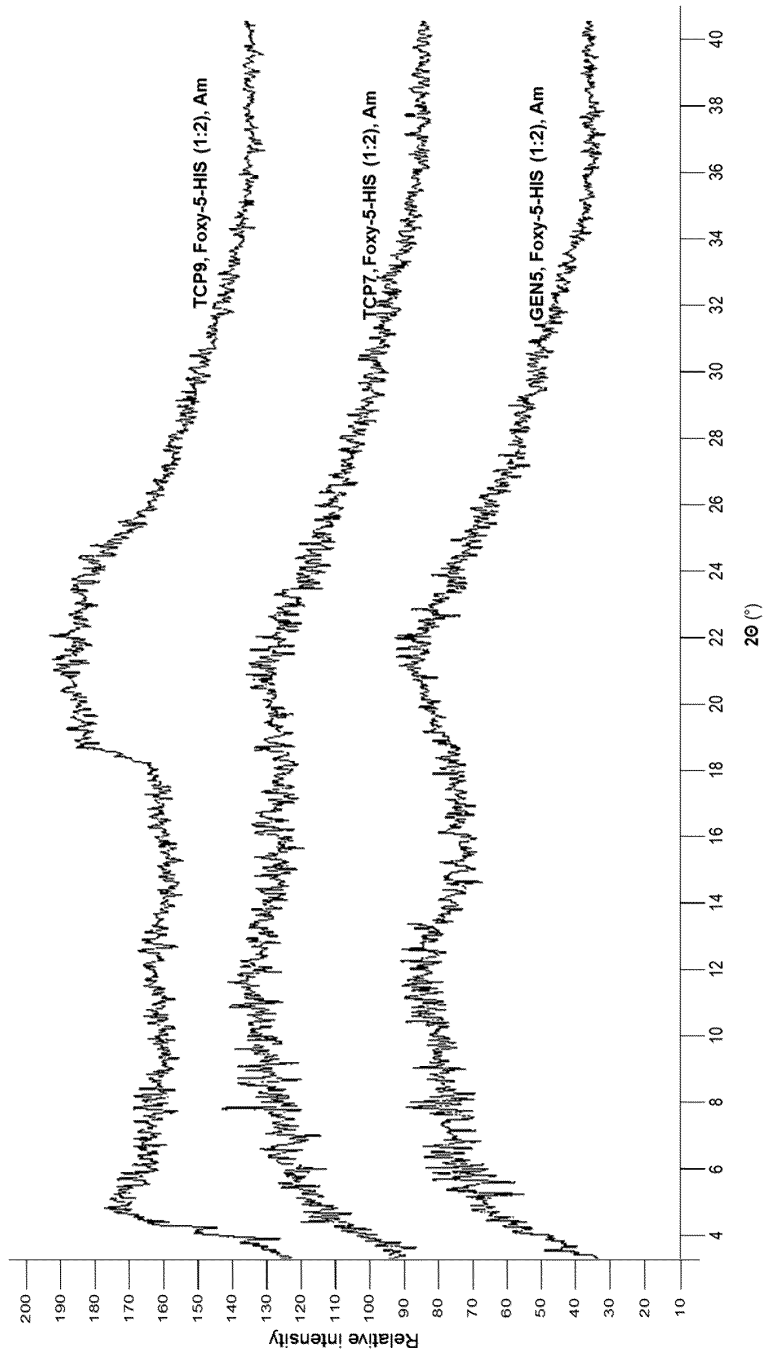


FIG.14

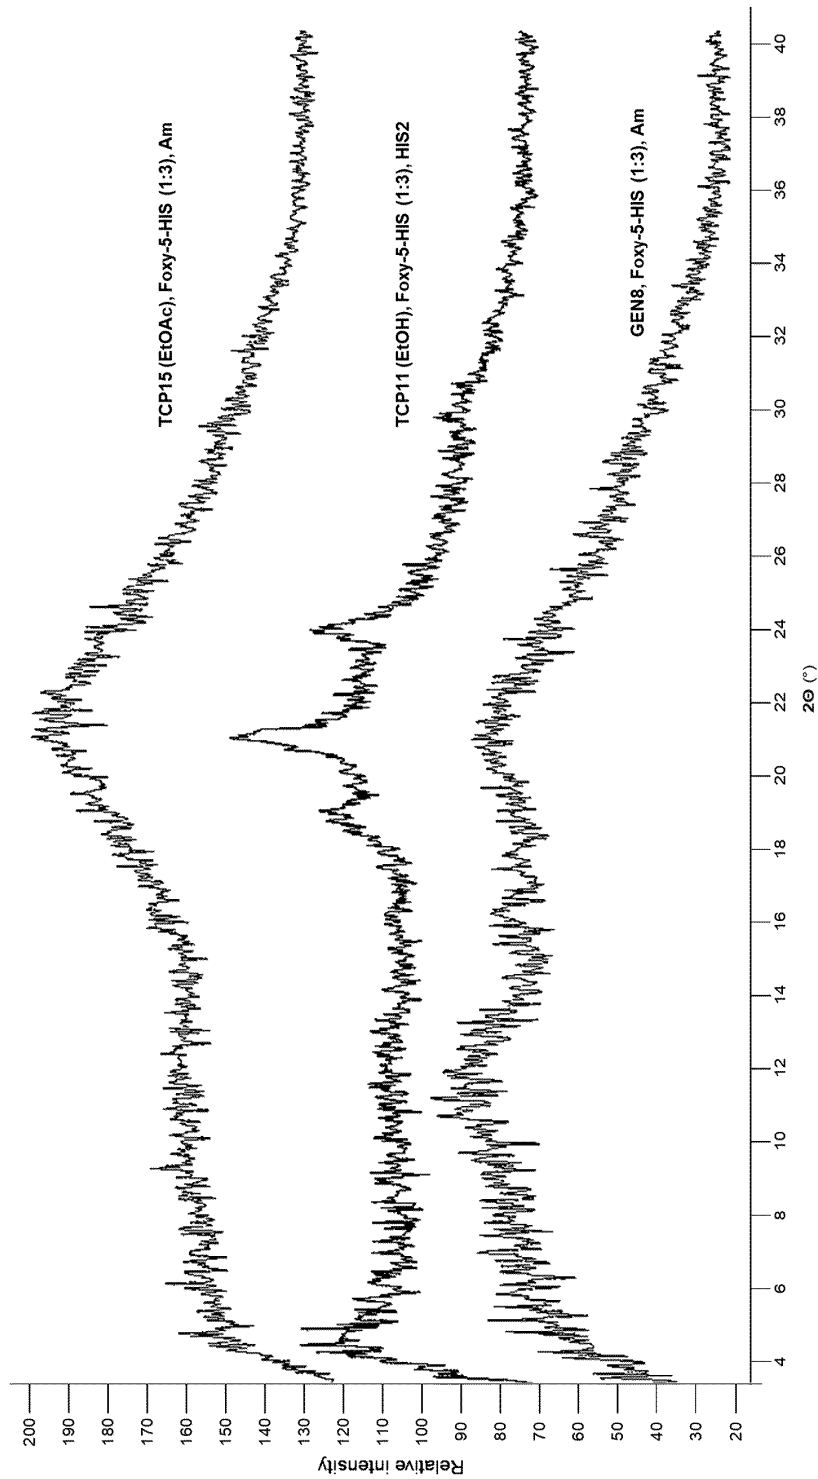


FIG.15

