

Schematic longitudinal cross-sectional view of catheter-deliverable device frame

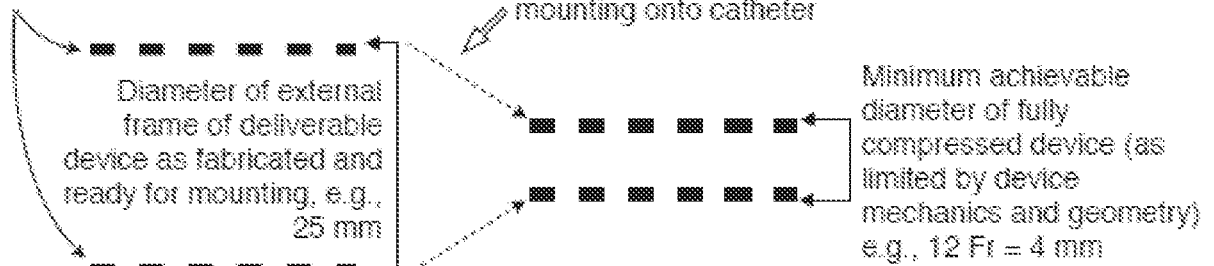


FIG. 1
(PRIOR ART)

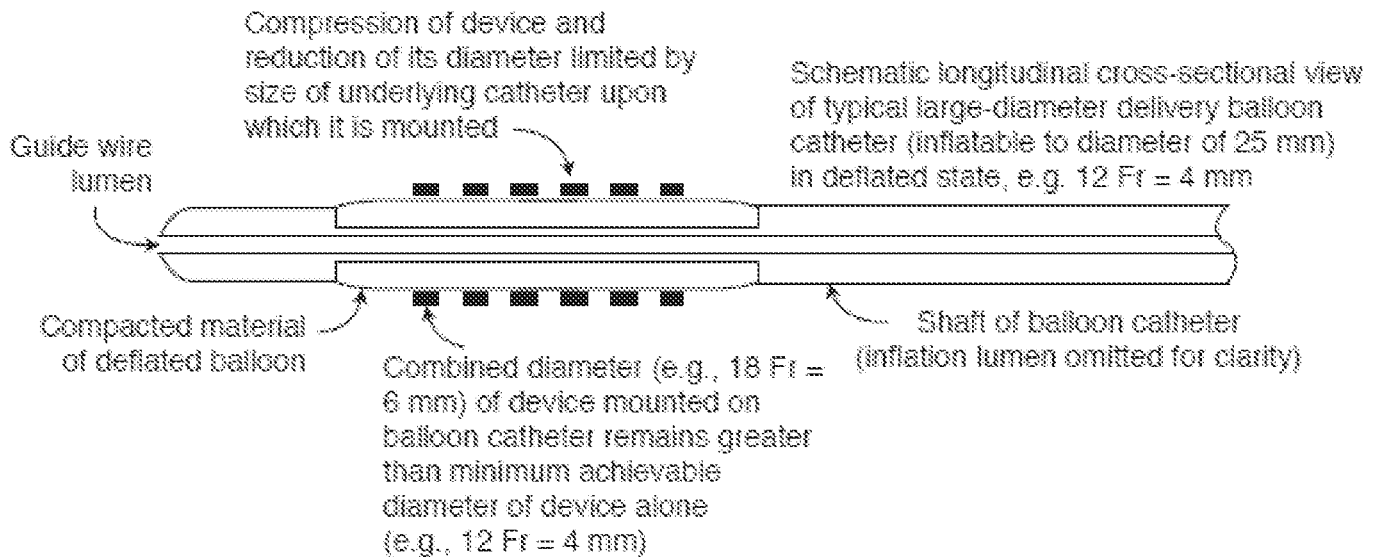


FIG. 2
(PRIOR ART)

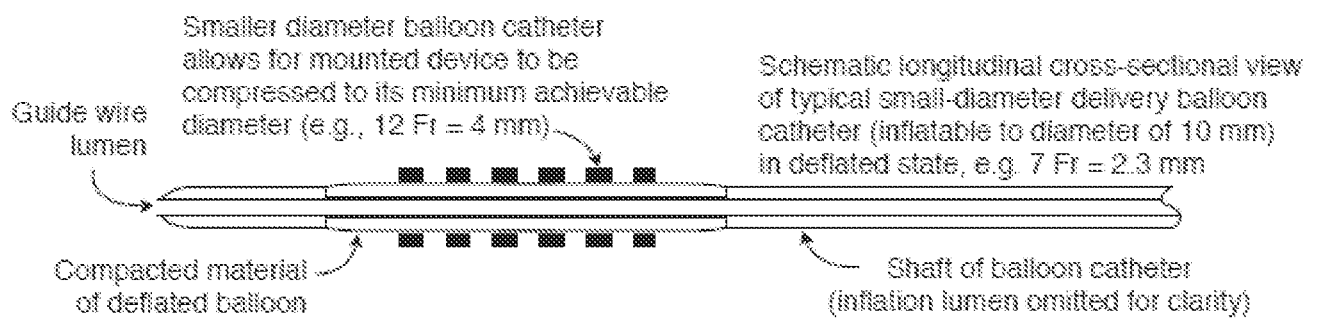


FIG. 3

FIG. 4A

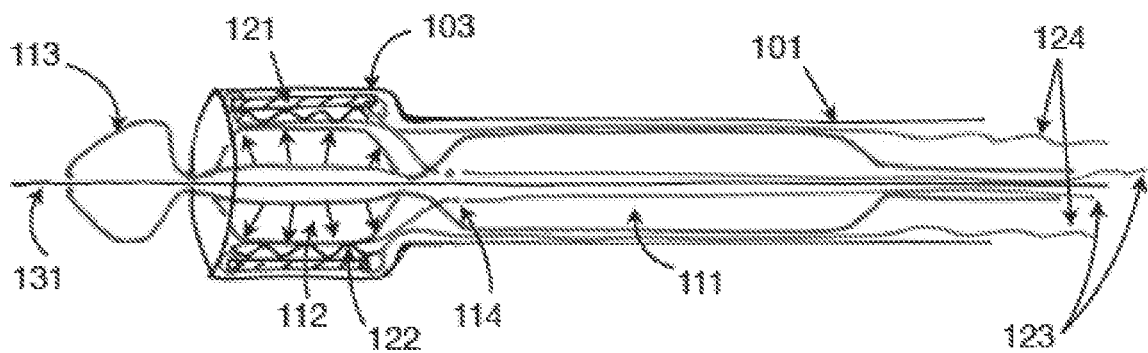
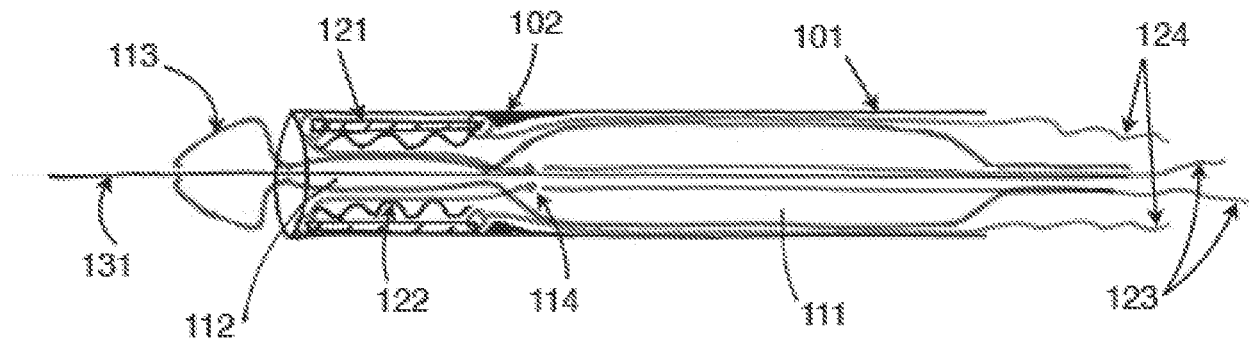


FIG. 4B

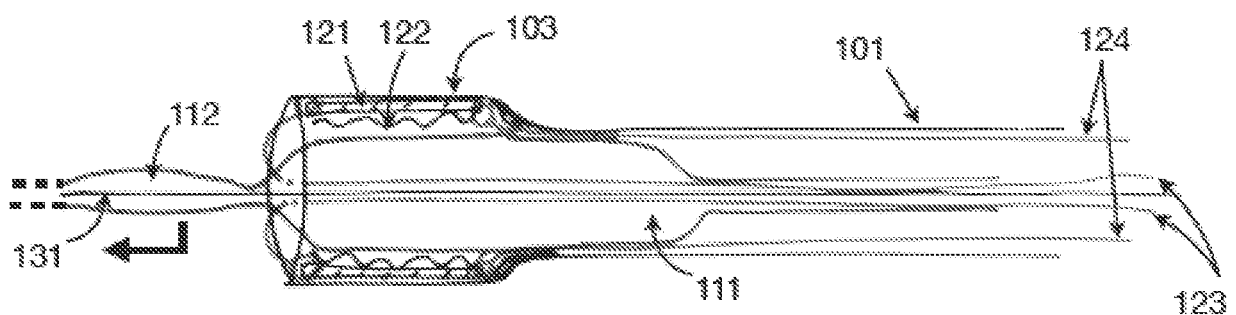


FIG. 4C

FIG. 4D

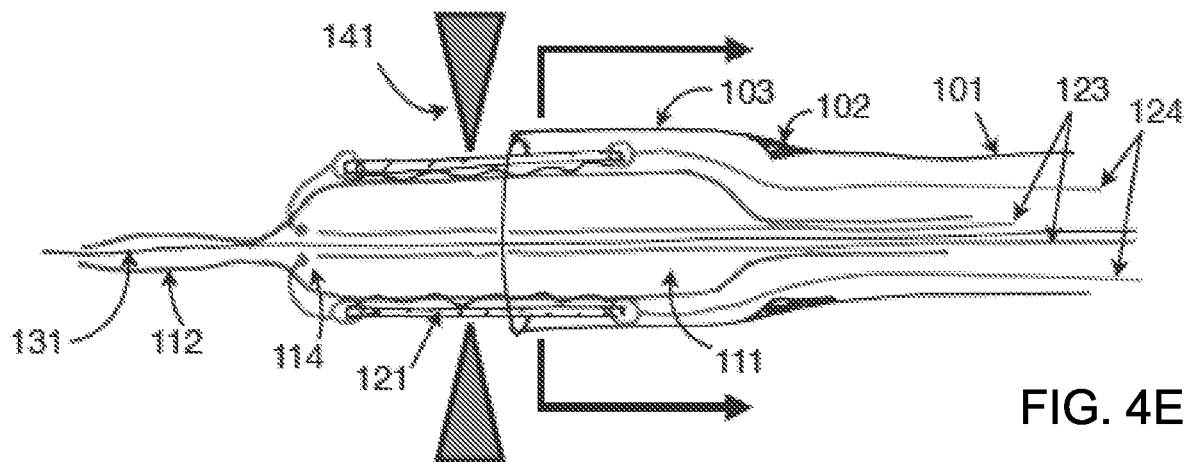
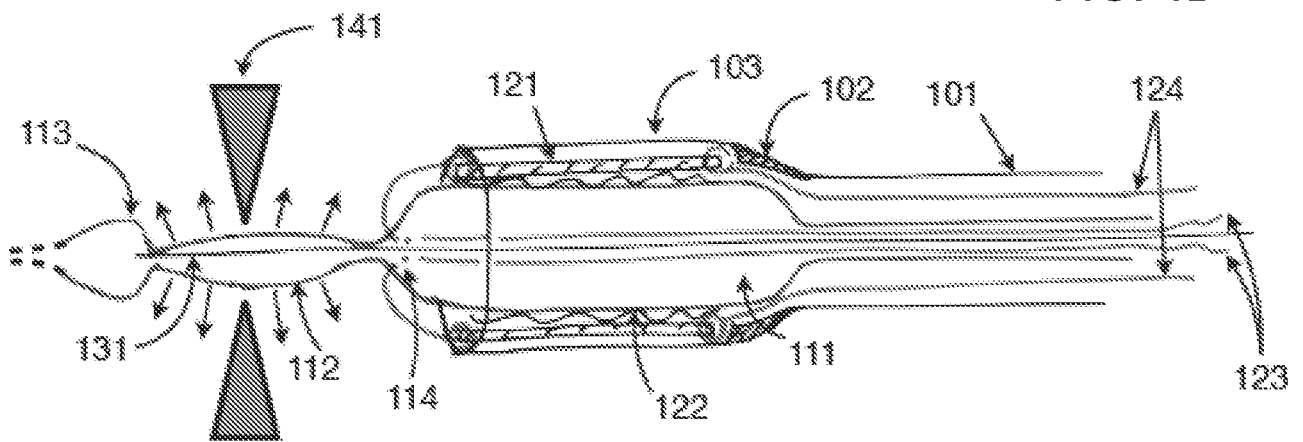


FIG. 4E

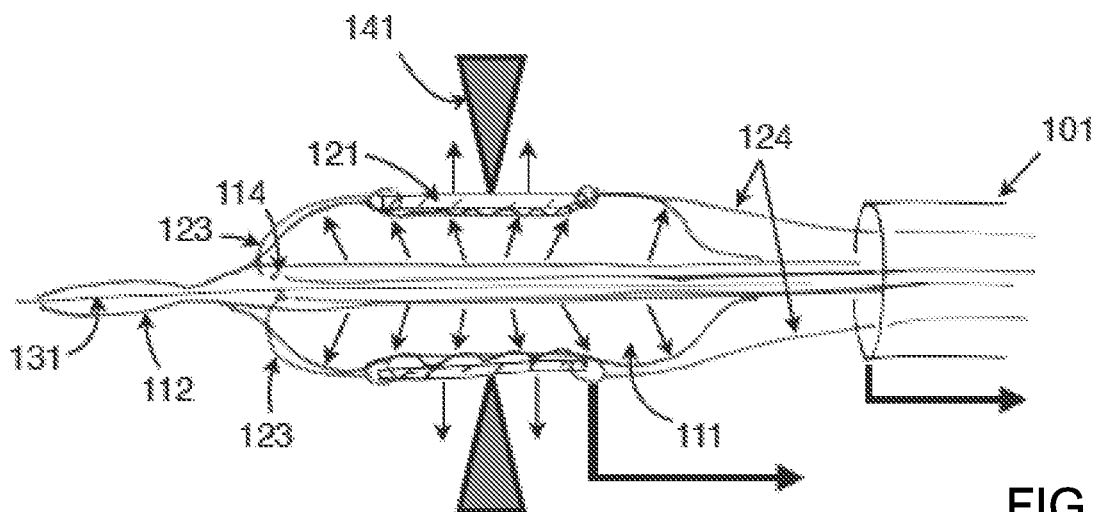


FIG. 4F

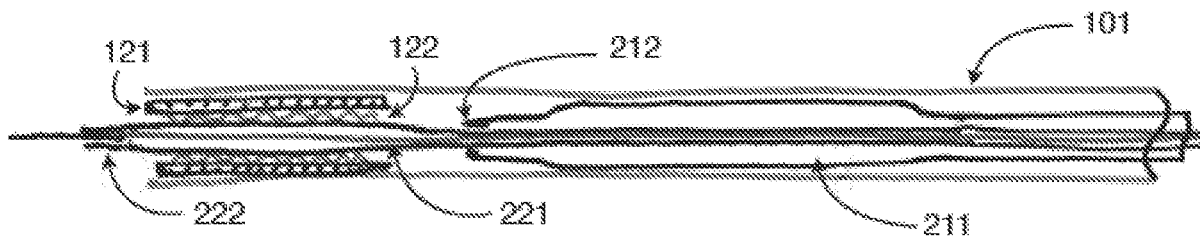


FIG. 5A

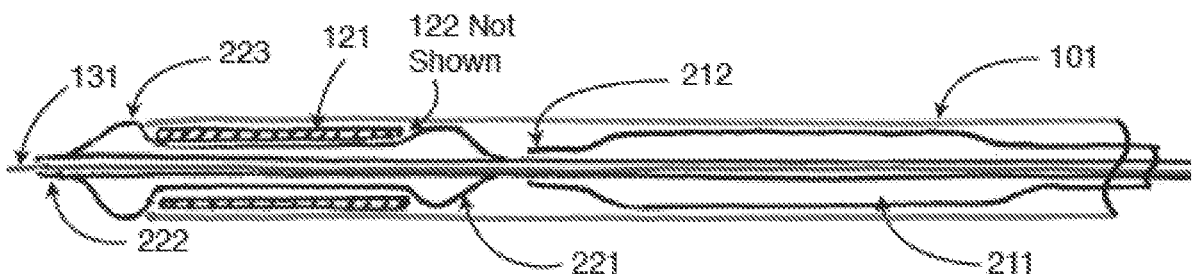


FIG. 5B

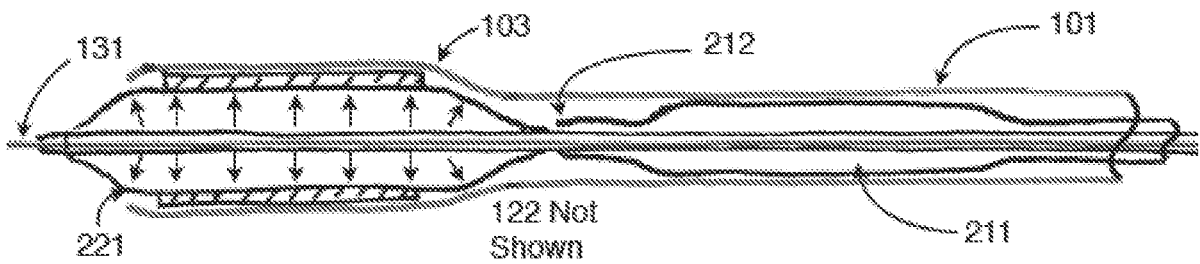


FIG. 5C


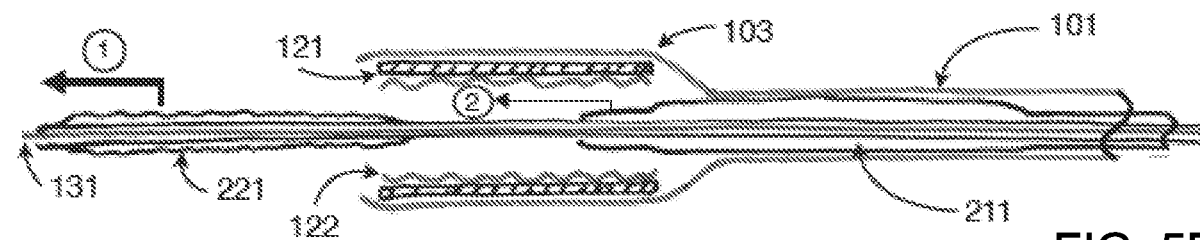


FIG. 5D

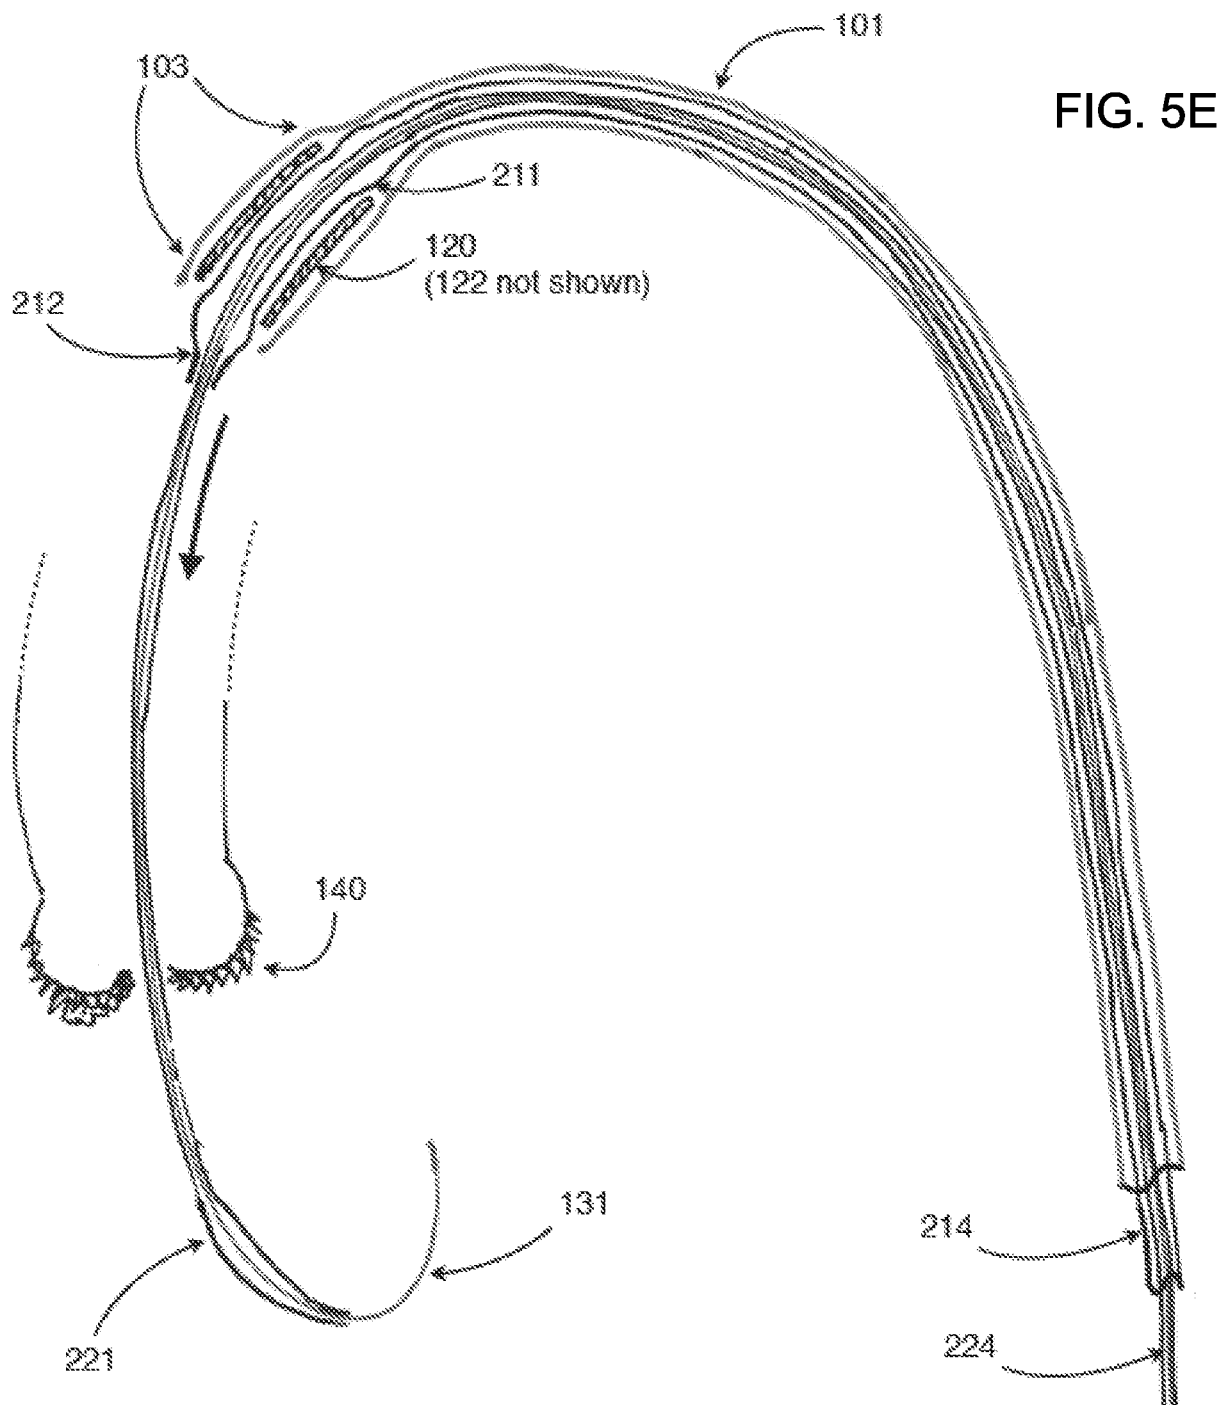

Proximal catheter ports
and hubs not shown

FIG. 6A

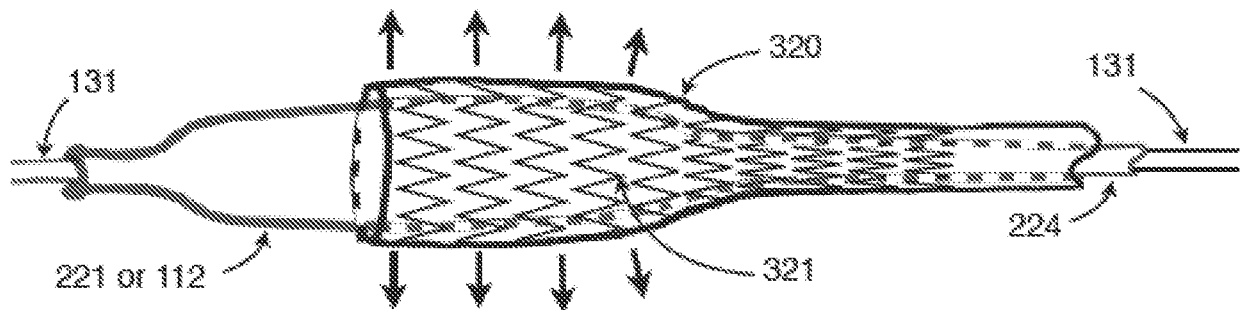
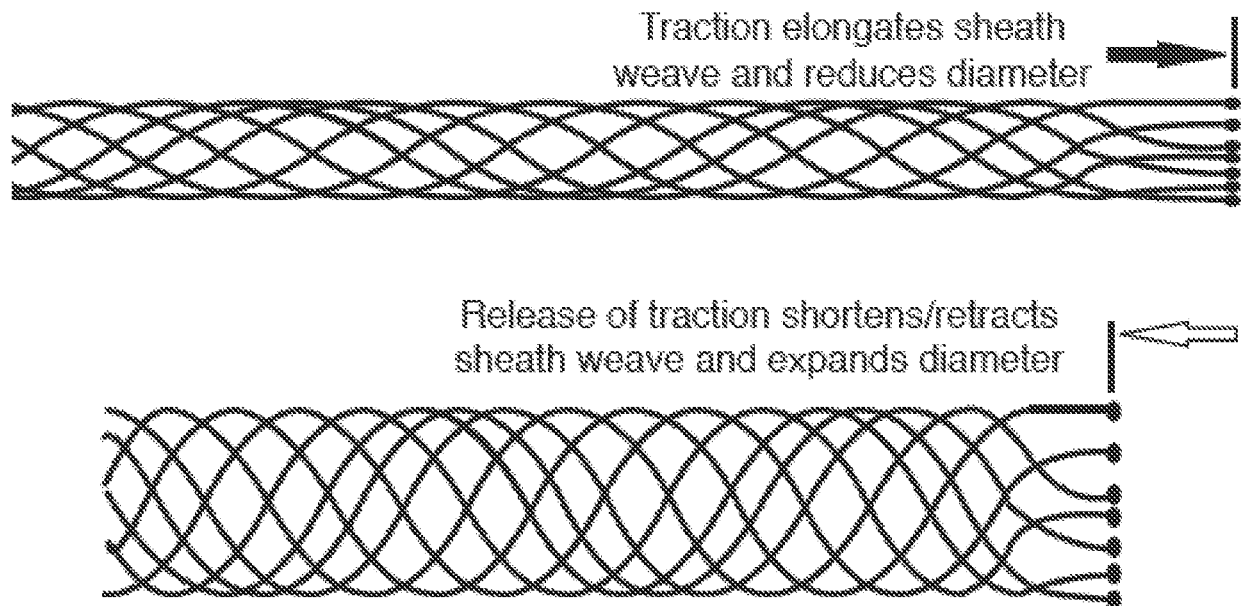


FIG. 6B

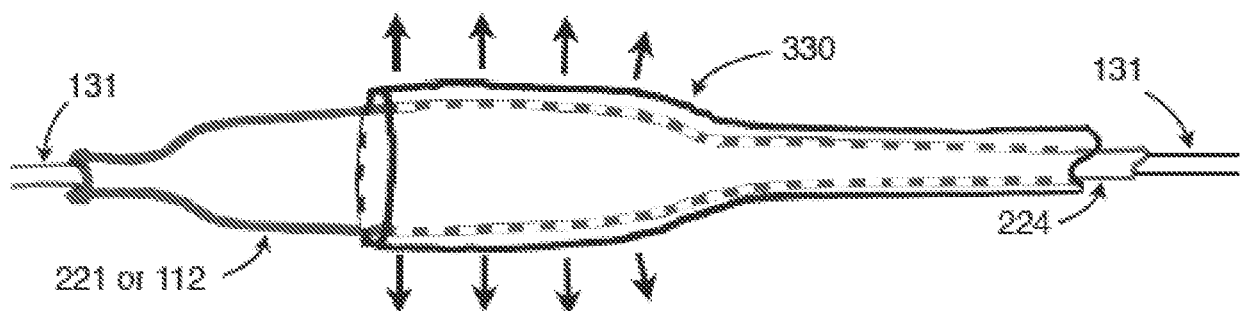


FIG. 6C

FIG. 6D

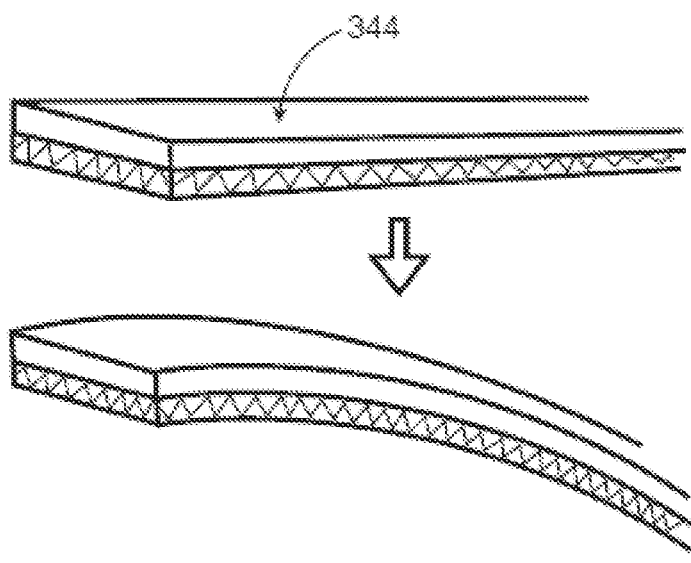
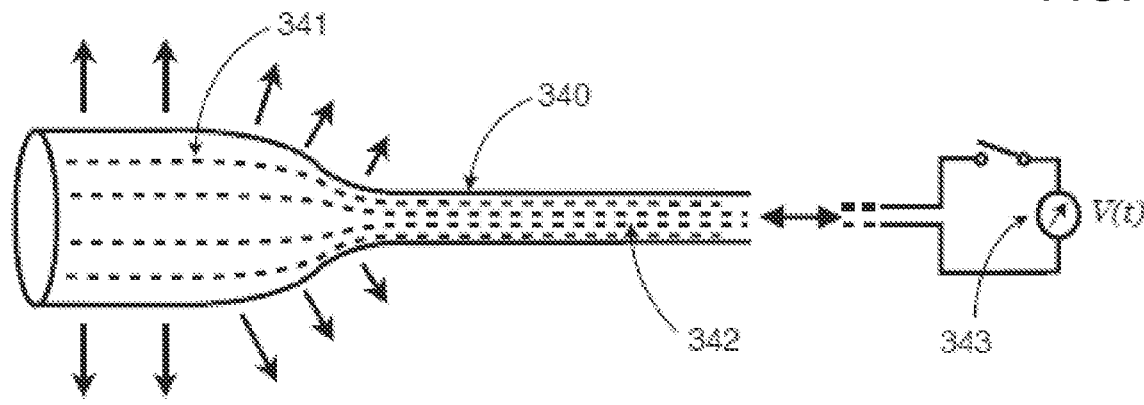


FIG. 6E

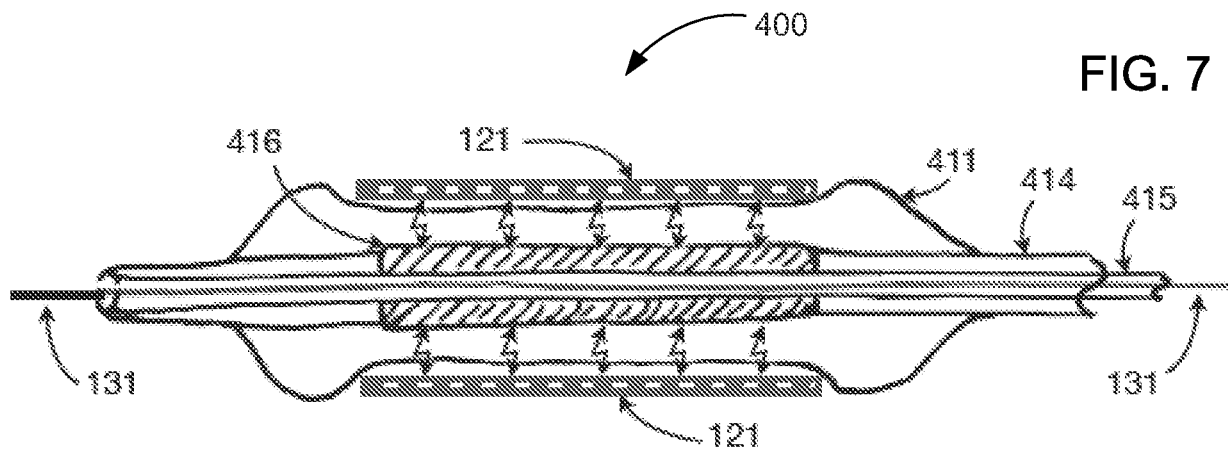


FIG. 7

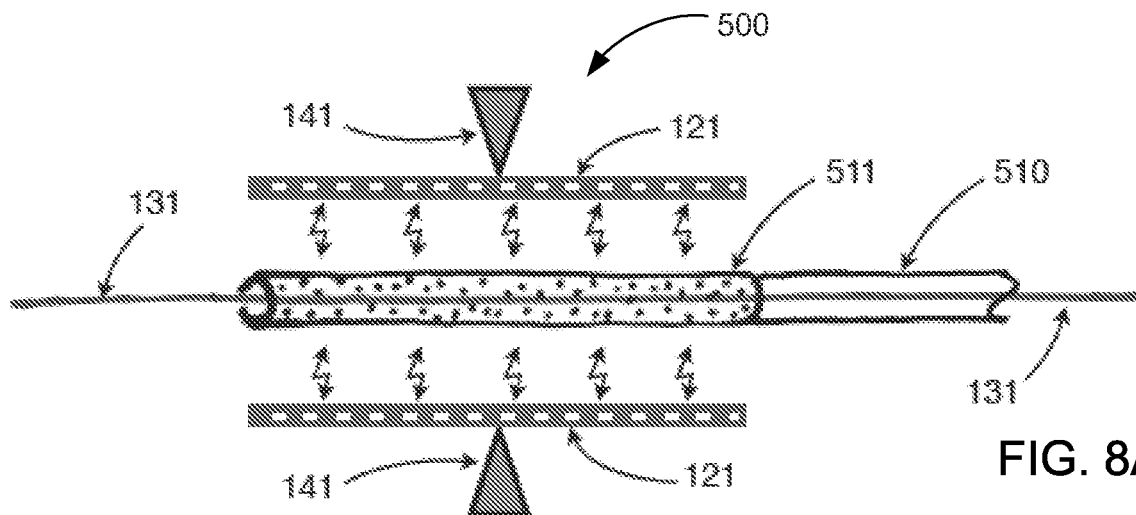


FIG. 8A

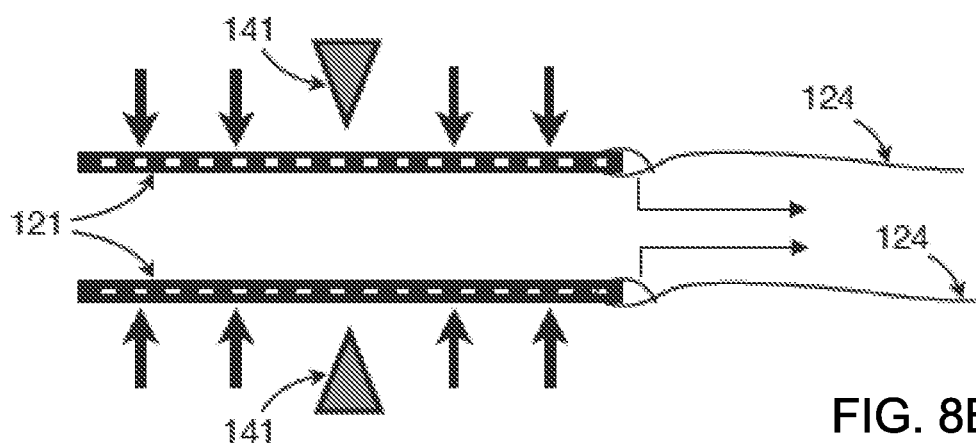


FIG. 8B

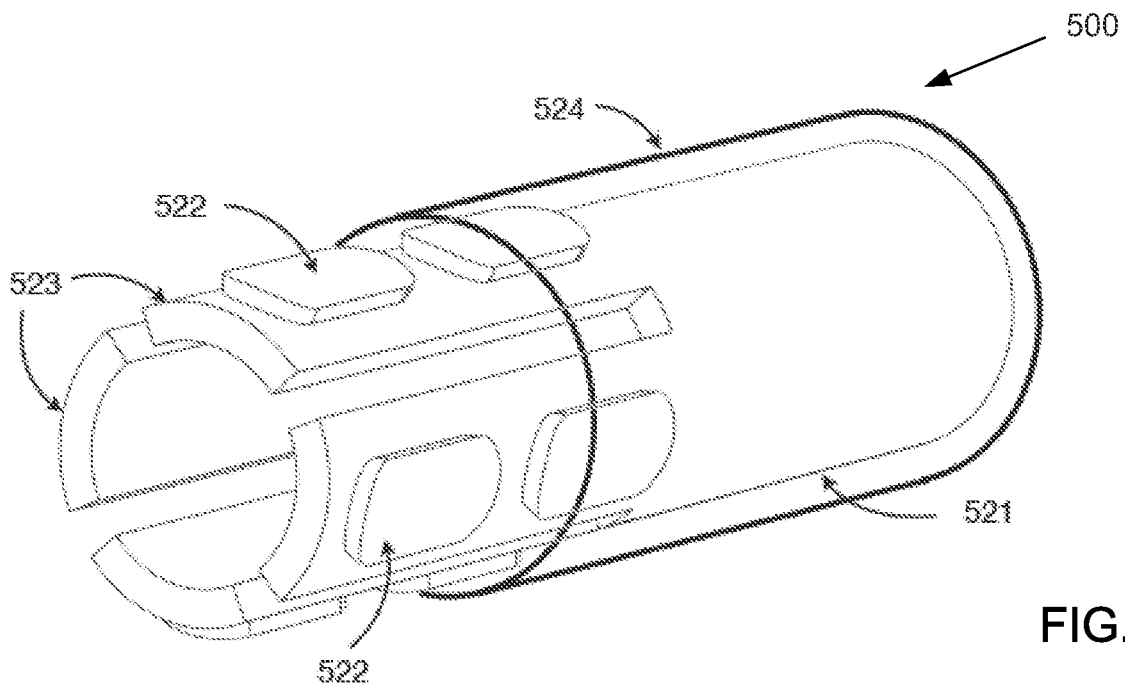


FIG. 8C

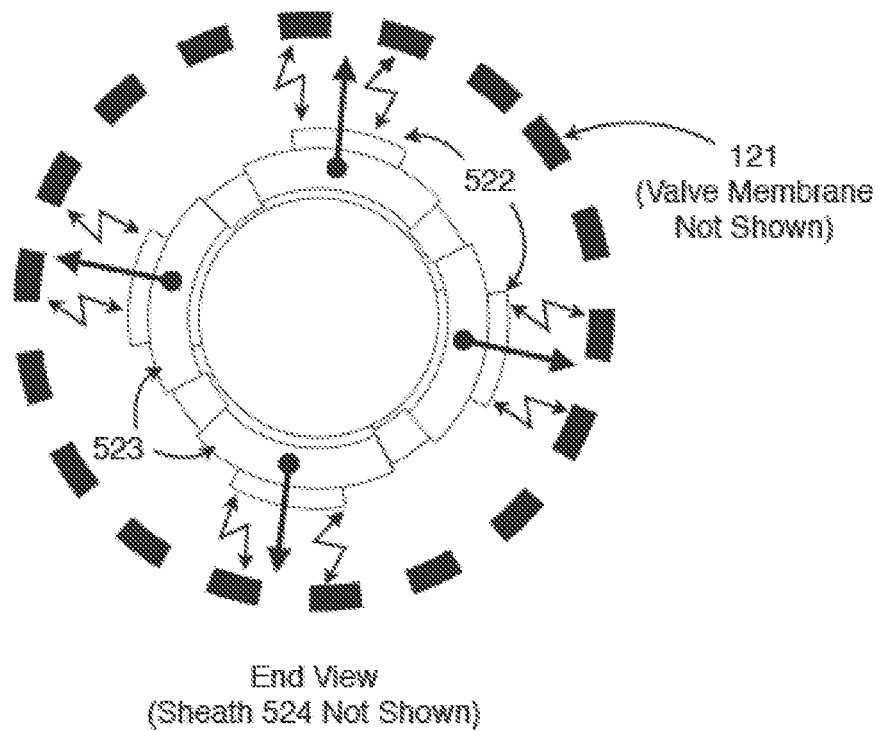


FIG. 8D