

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
15 December 2005 (15.12.2005)

PCT

(10) International Publication Number
WO 2005/118428 A1

(51) International Patent Classification⁷: **B65D 83/14**,
A61M 15/00, G01B 11/10

(21) International Application Number:
PCT/SE2005/000825

(22) International Filing Date: 1 June 2005 (01.06.2005)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
0401408-0 2 June 2004 (02.06.2004) SE

(71) Applicant (for all designated States except US): **ASTRAZENECA AB** [SE/SE]; S-151 85 Södertälje (SE).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **METCALE, Stephen** [GB/GB]; AstraZeneca R & D Charnwood,

Bakewell Road, Loughborough Leicestershire LE11 5RH (GB). **FLETCHER, Ian** [GB/GB]; AstraZeneca R & D Charnwood, Bakewell Road, Loughborough Leicestershire LE11 5RH (GB).


(74) Agent: **DR LUDWIG BRANN PATENTBYRÅ AB**; c/o AstraZeneca R & D Södertälje, S-151 85 Södertälje (SE).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SM, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH,

[Continued on next page]

(54) Title: DIAMETER MEASURING DEVICE

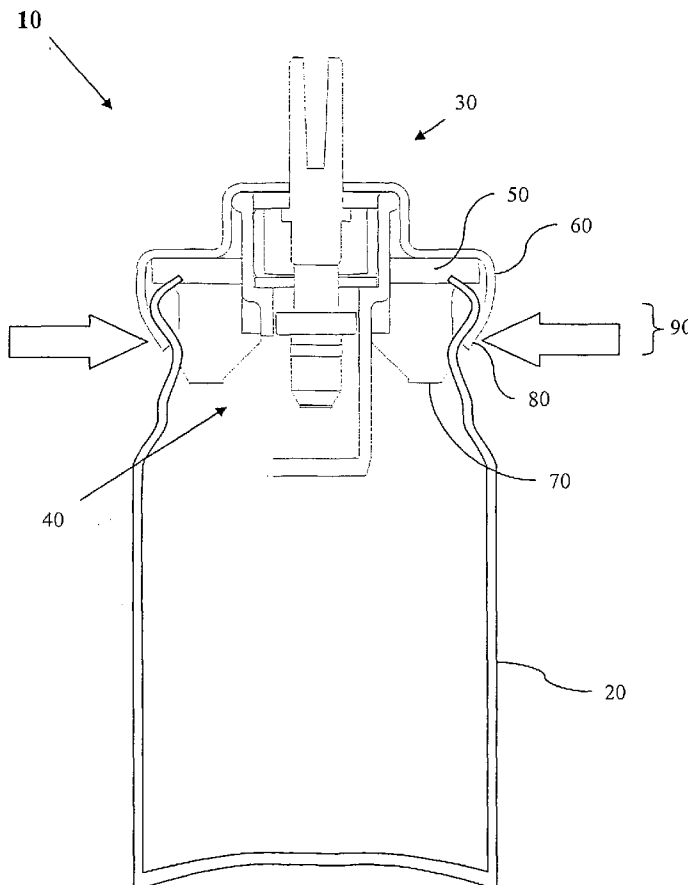

(57) Abstract: Method of detecting a potentially void inhaler can valve (30), which valve (30) is attached to a can (10) by a ferrule crimp (80), comprising the steps: placing the can (10) in a can jig (220) that is arranged to retain the can (10) at a predetermined measurement height with respect to a diameter measuring means (230), measuring the diameter of the ferrule crimp (80) at the predetermined height, and comparing the measured crimp diameter with a predefined interval of acceptance, and if the measured diameter is outside a predefined interval classifying the inhaler can valve (30) as potentially void. There is also provided a crimp diameter measuring device (200) comprising: a base (210), a diameter measuring means (230) supported by the base (210), and a can jig (220) supported by the base (210), the can jig (220) being arranged to retain a can (10) placed therein at a predetermined measurement height with respect to a diameter measuring means (230).



GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report*

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.