

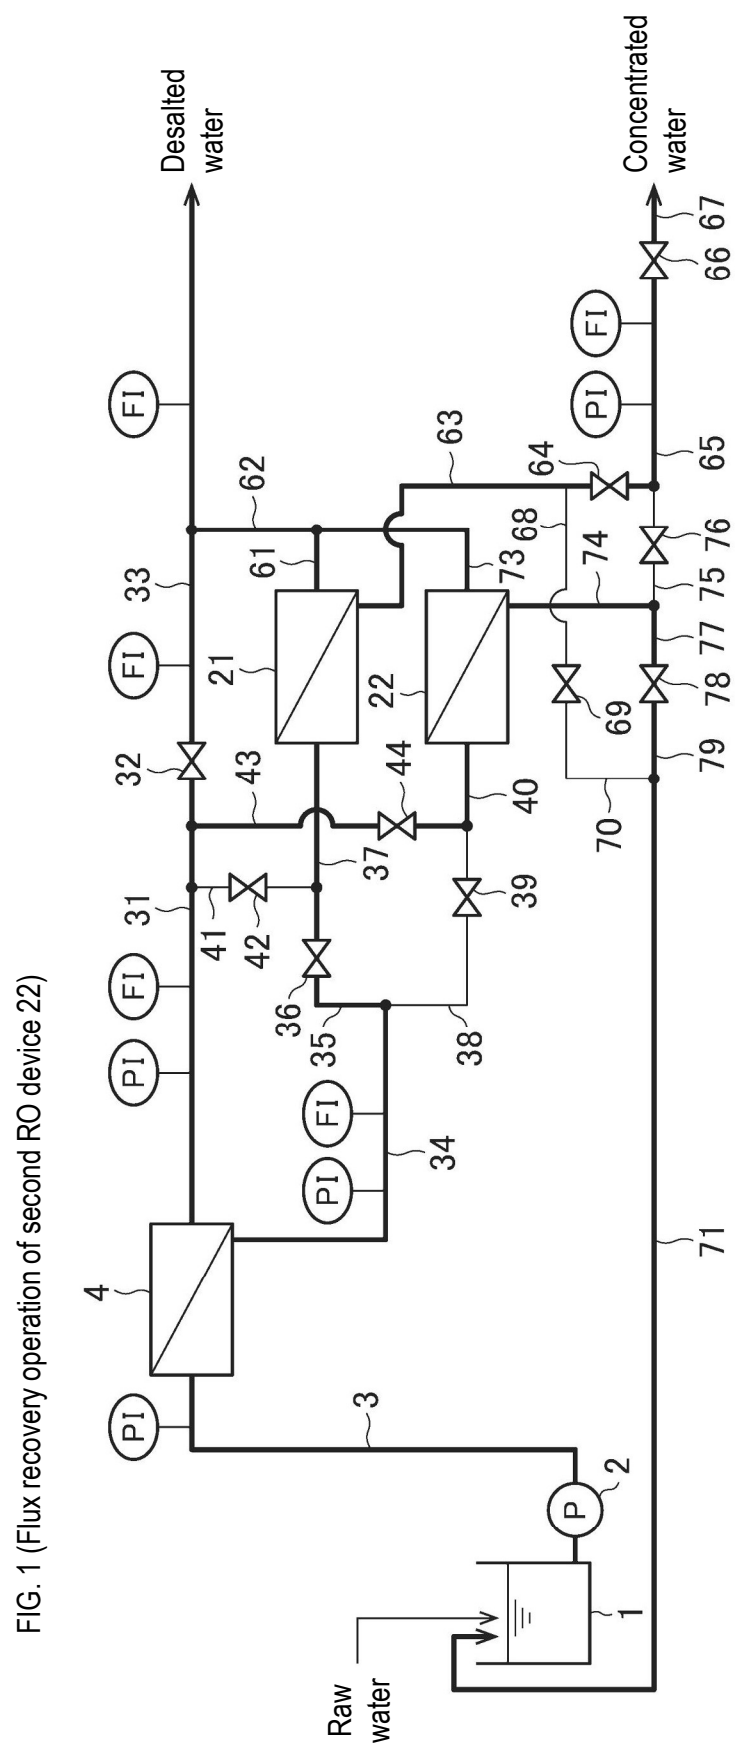


FIG. 1

FIG. 2 (Flux recovery operation of second RO device 21)

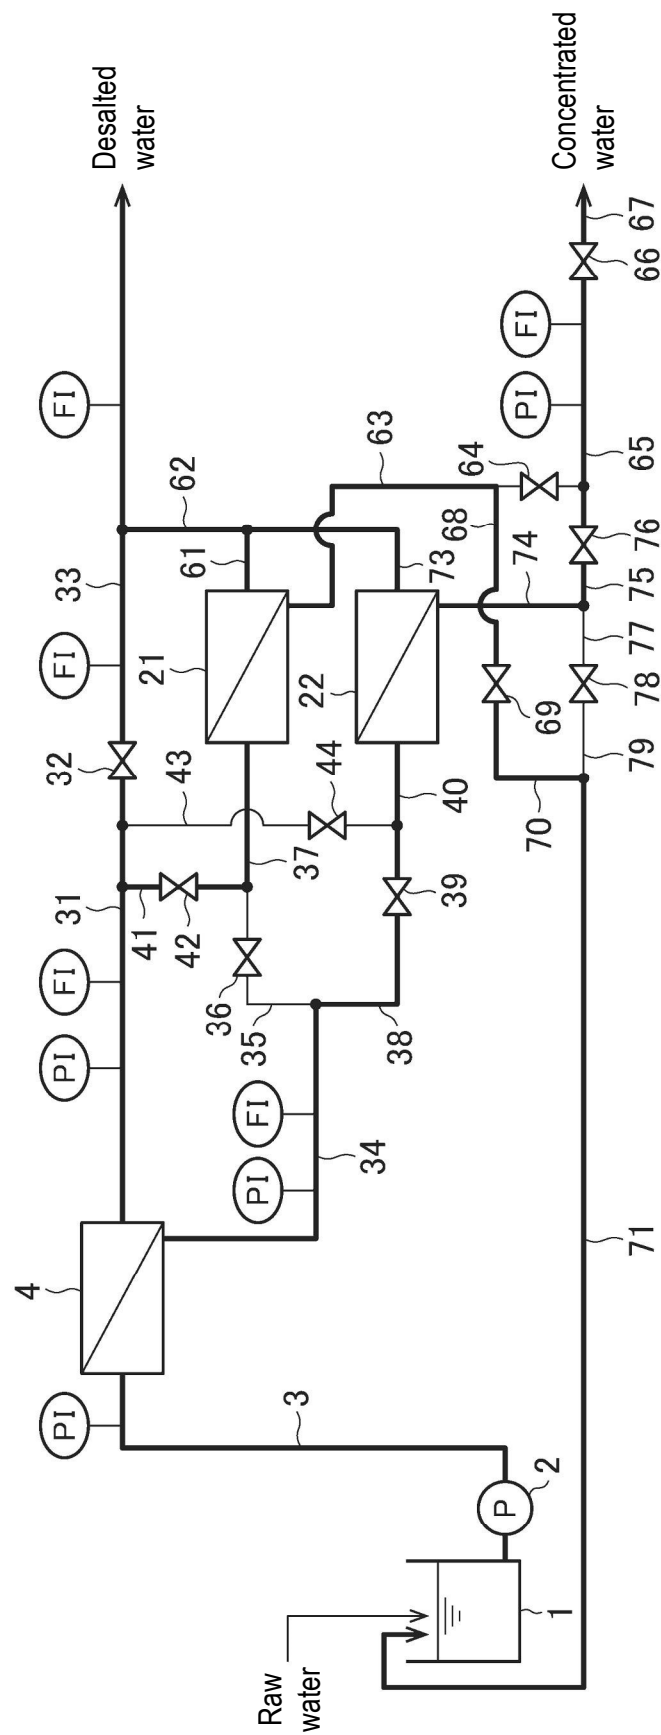
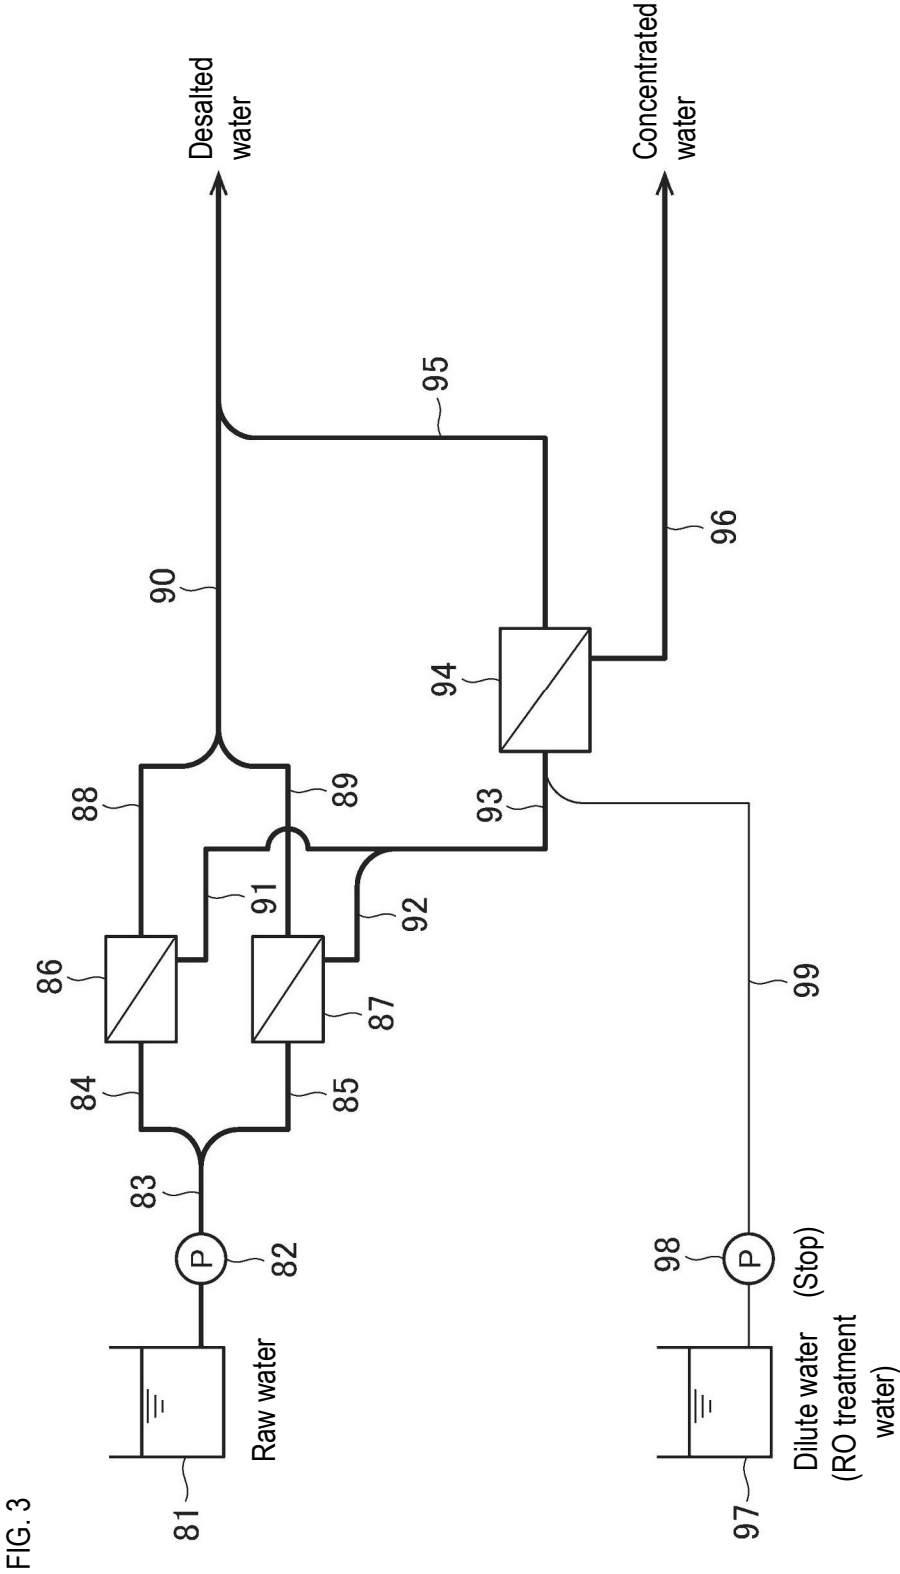


FIG. 2



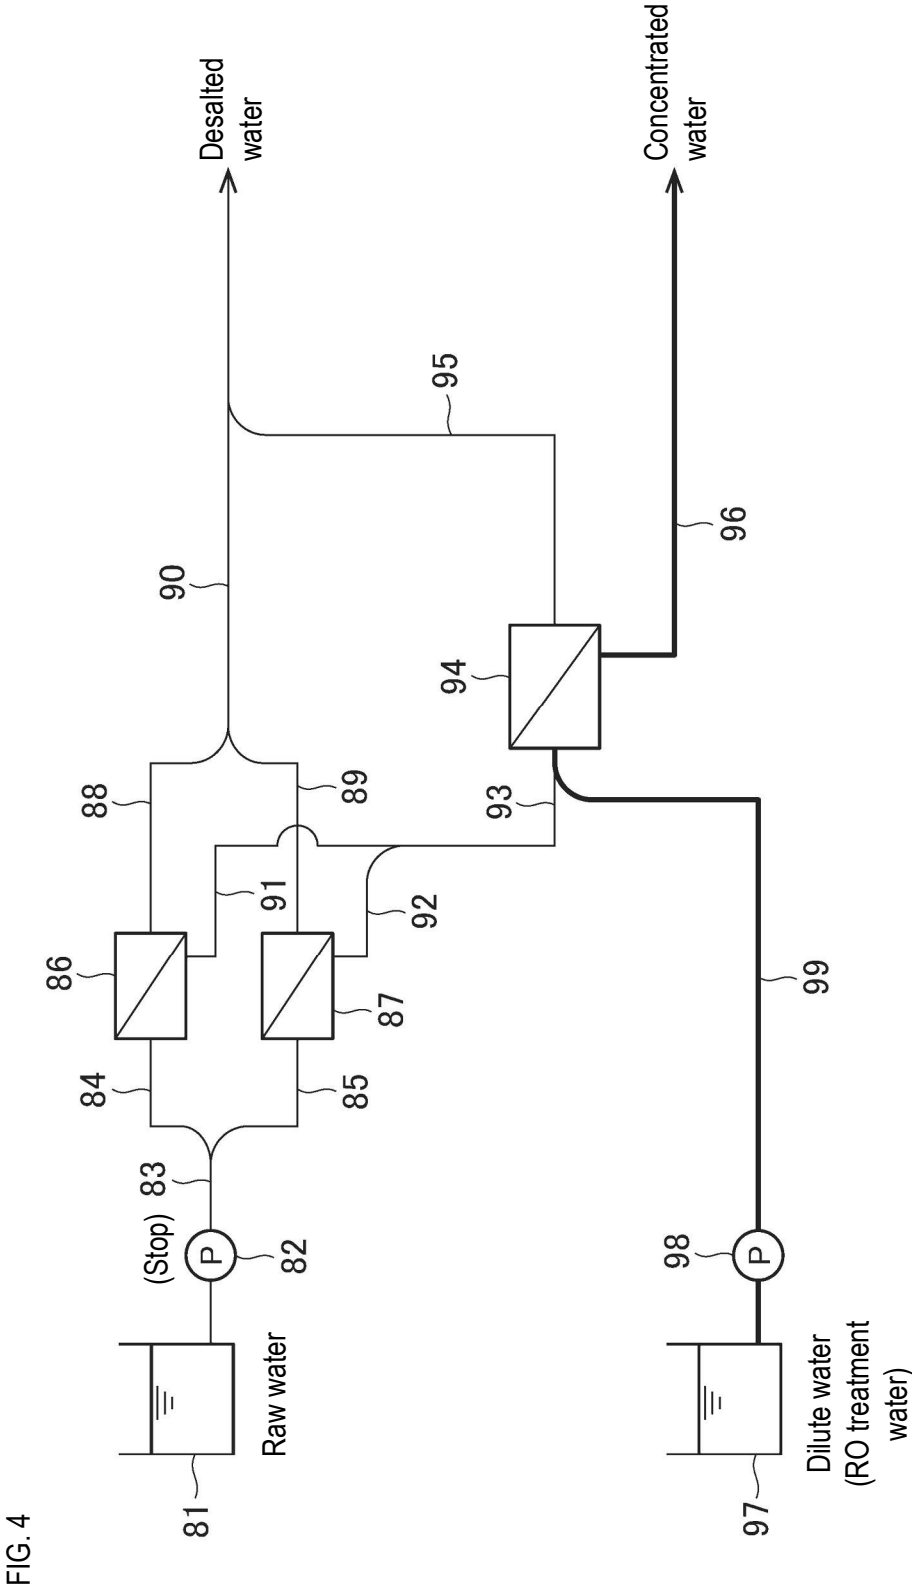


FIG. 5

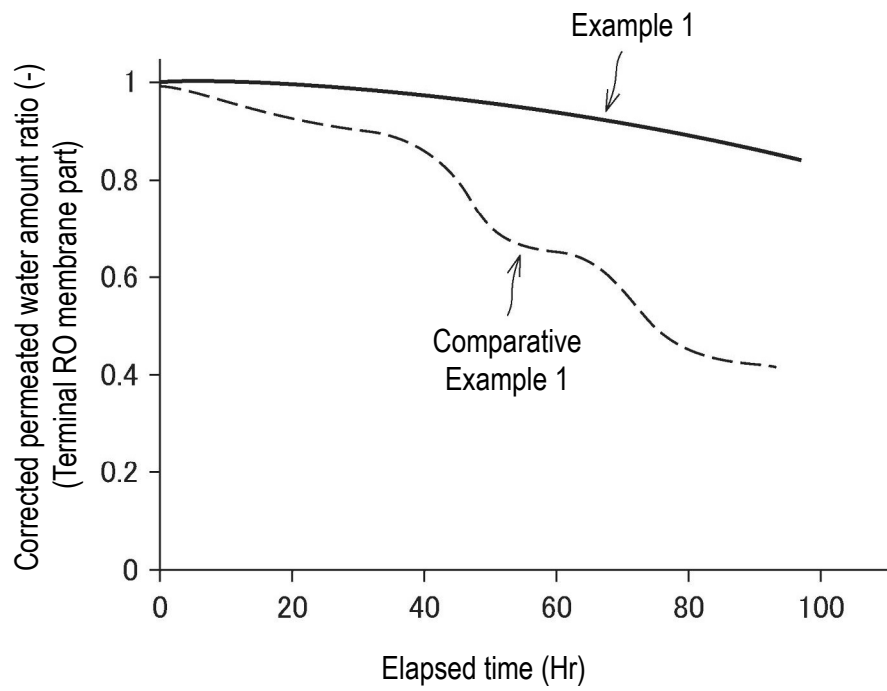


FIG. 5