

FIG. 1
Time/Mortality Response of Susceptible and Resistant *Aedes aegypti* to
Permethrin in Bottle Bioassay

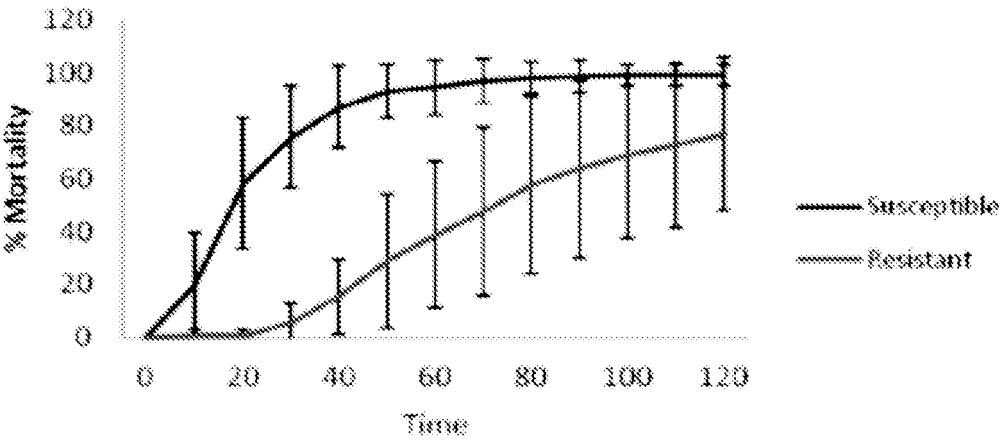


FIG. 2

Time/Mortality Response of Susceptible and Resistant *Aedes aegypti* to C8910 in Bottle Bioassay

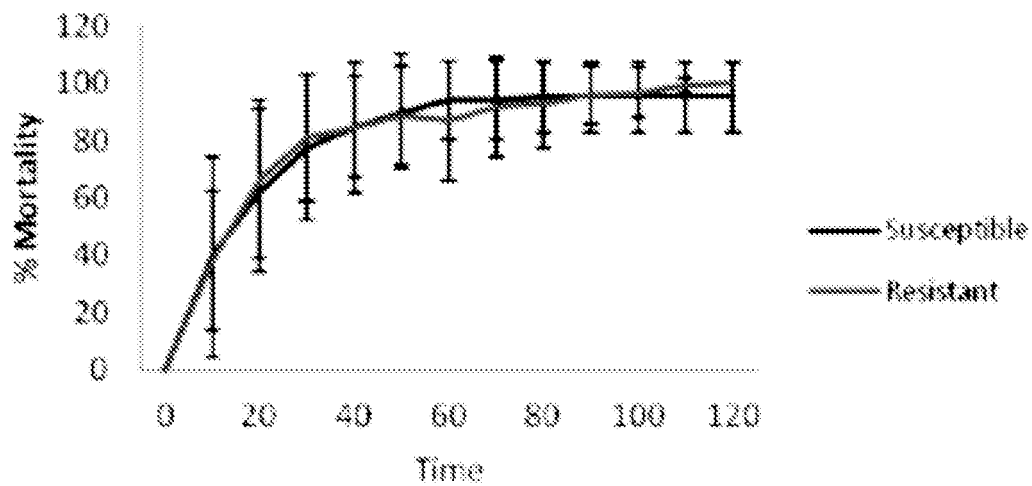


FIG. 3

Time/Mortality Response of Susceptible and Resistant *Aedes aegypti* to a 1:0.01 ratio of C8910 with Permethrin in Bottle Bioassay

