

FIG. 1

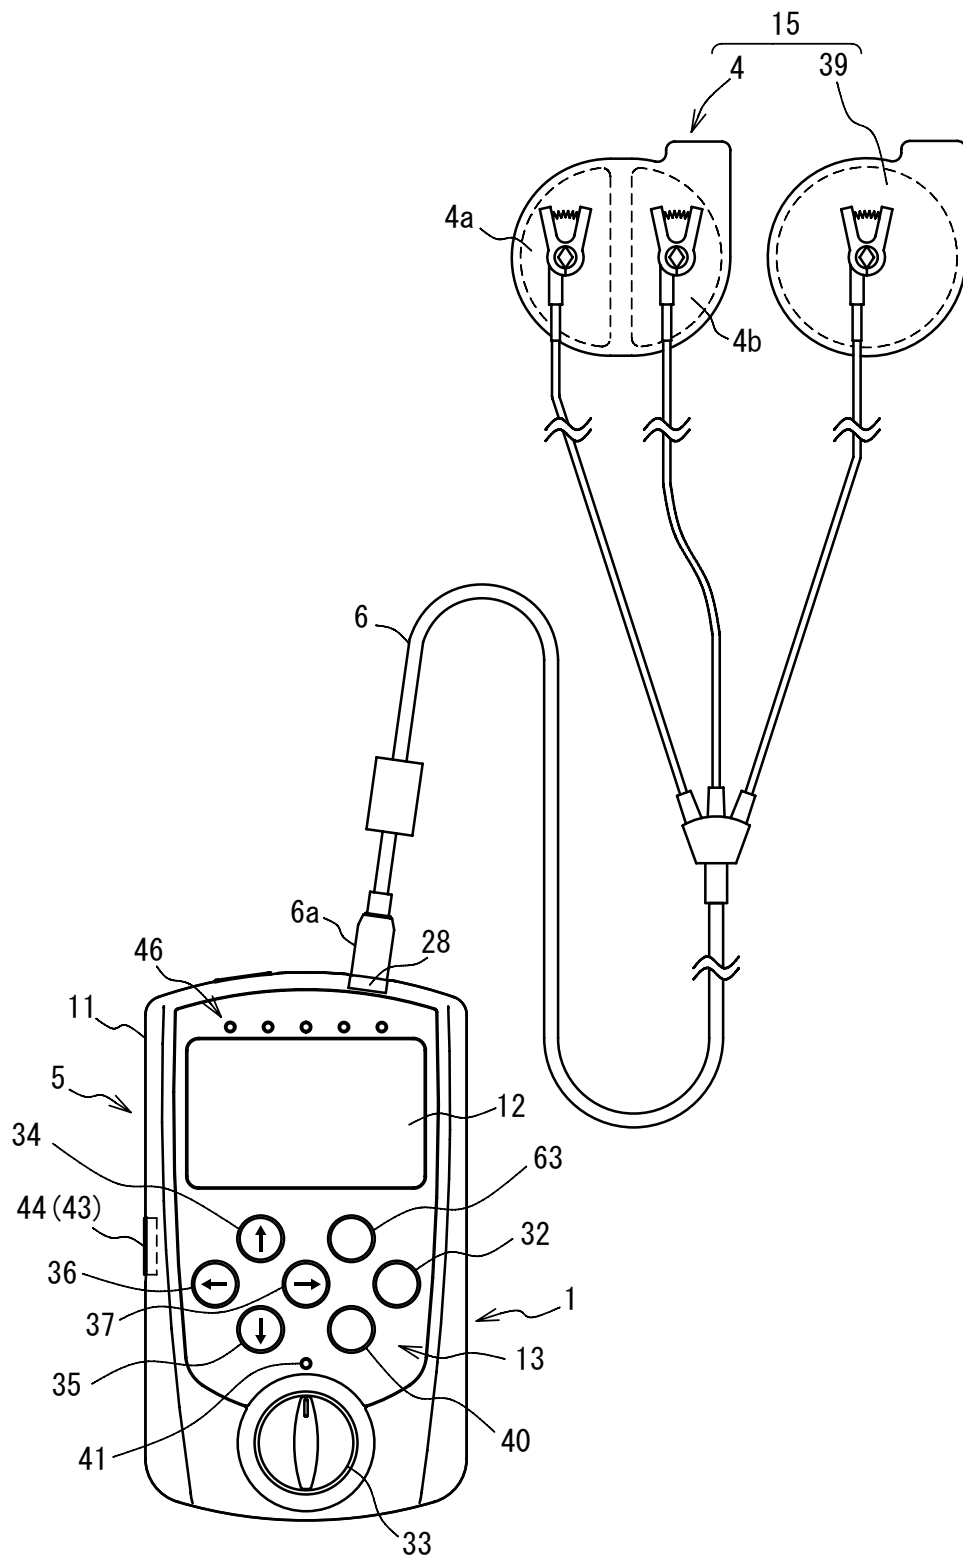


FIG. 2

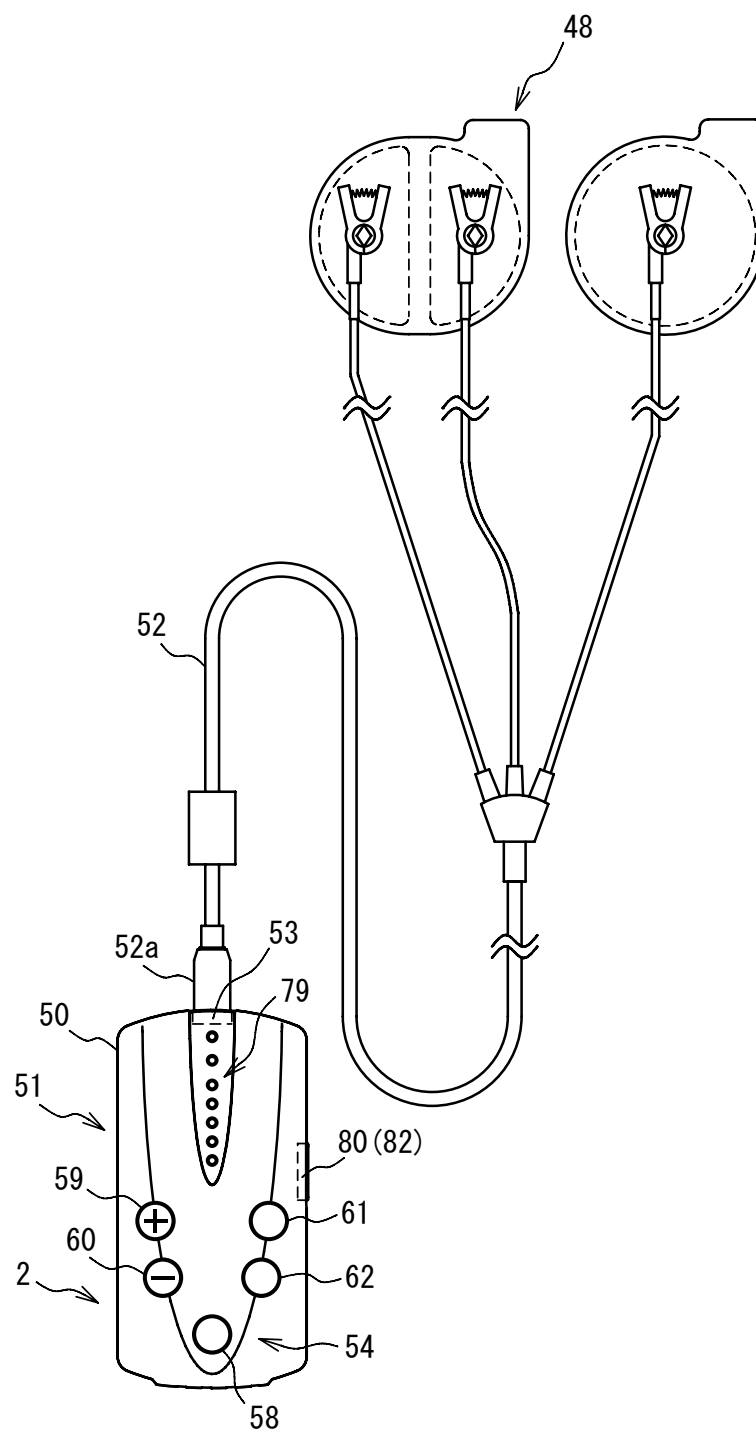


FIG. 3

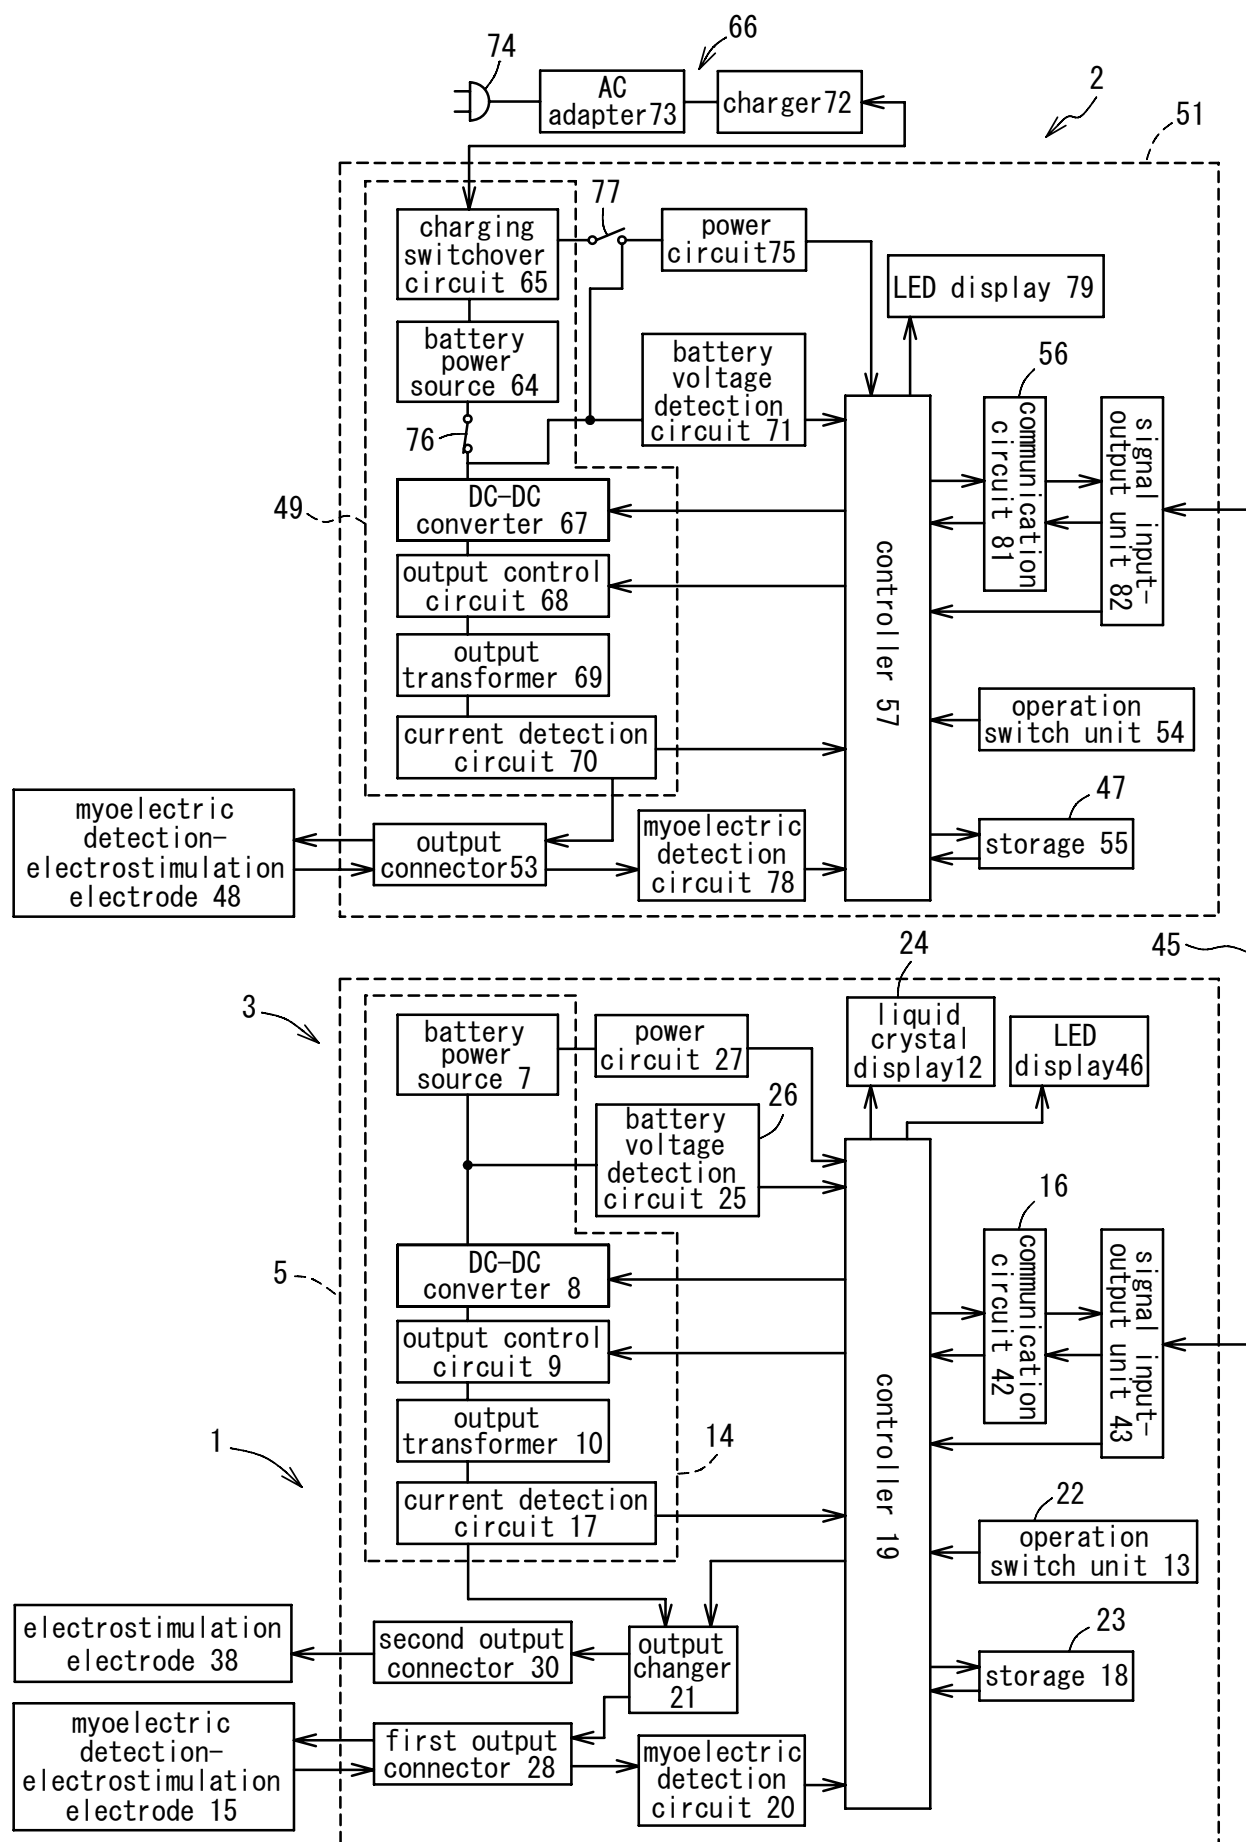


FIG. 4

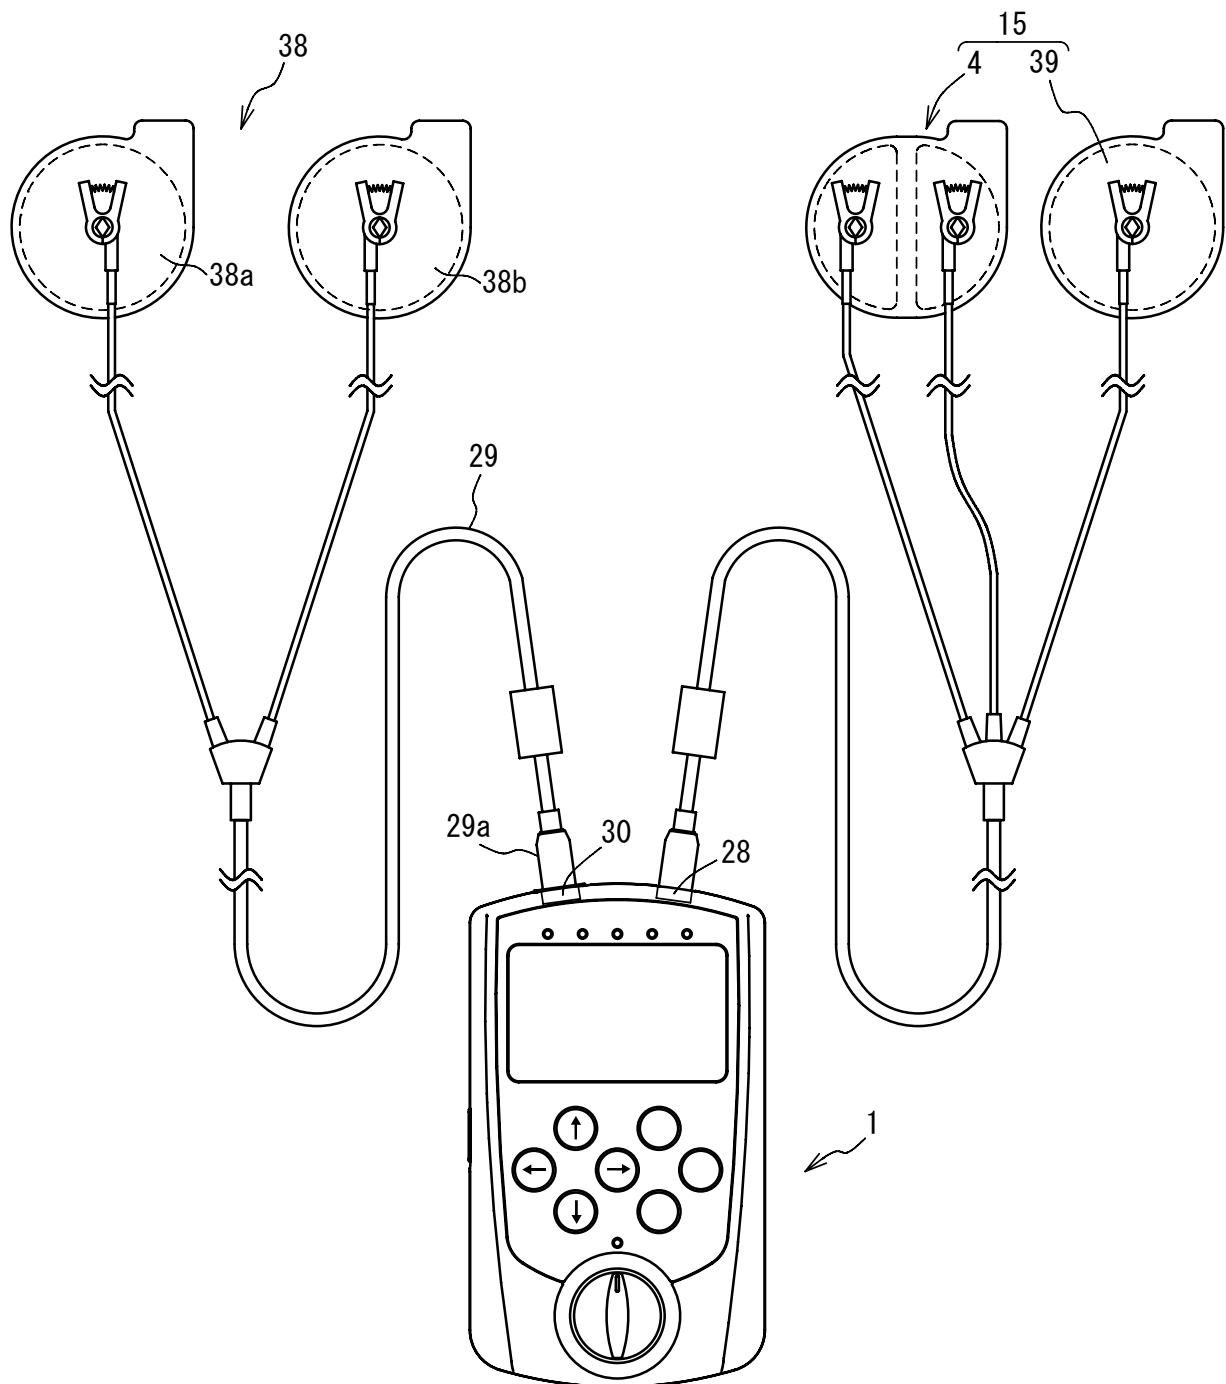


FIG. 5

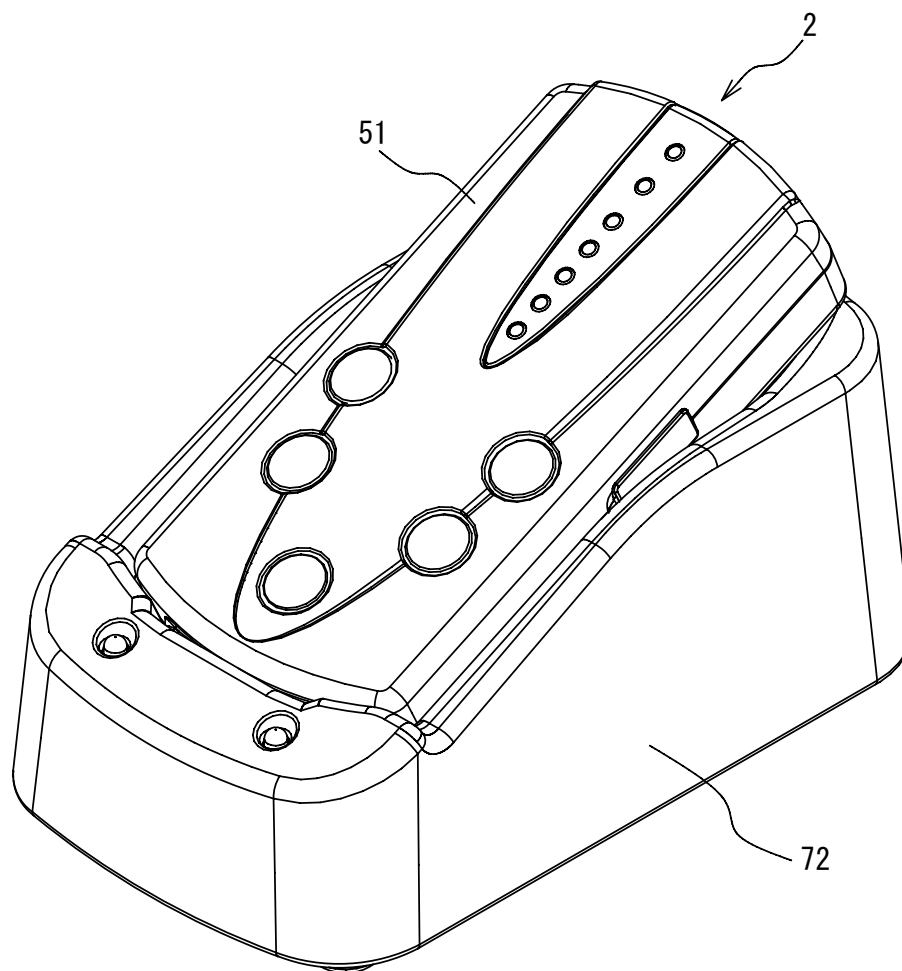


FIG. 6

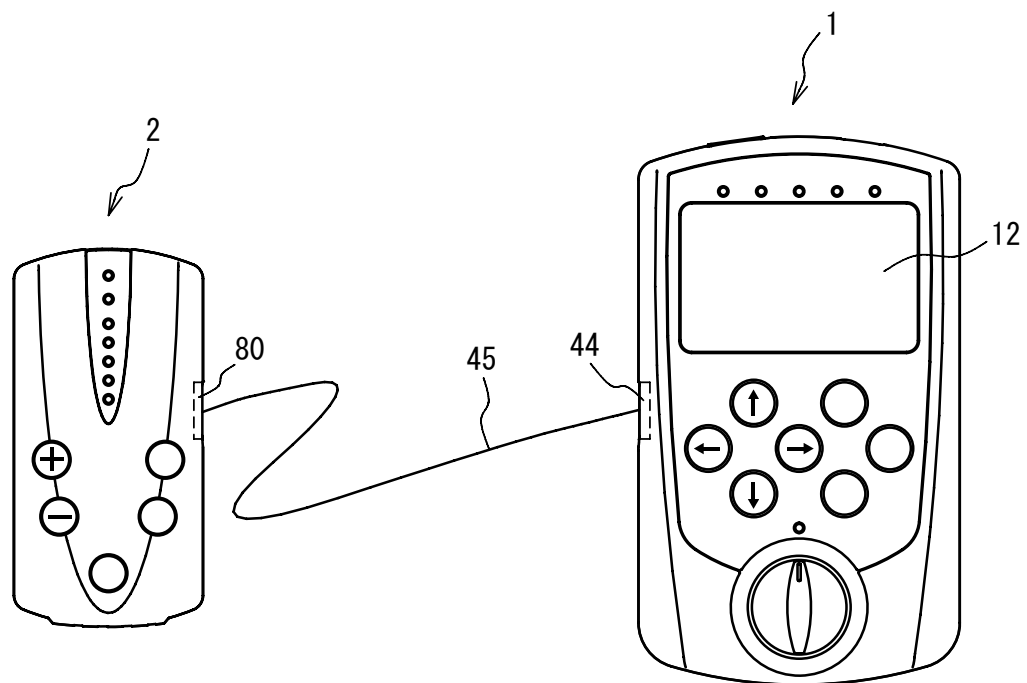


FIG. 7

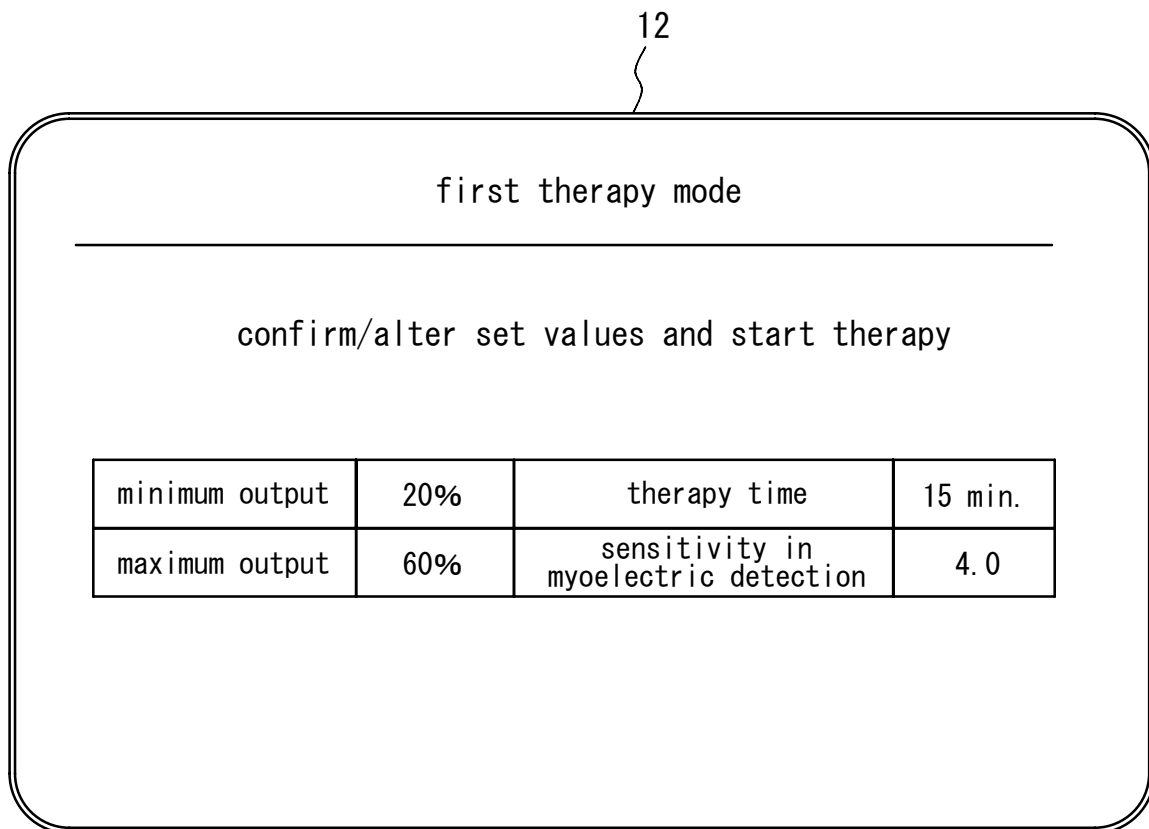


FIG. 8

12

confirm/alter and transmit set values

mode	first therapy mode		
minimun output	10%	therapy time	20 min.
maximum output	50%	sensitivity in myoelectric detection	3.5

transmit

FIG. 9

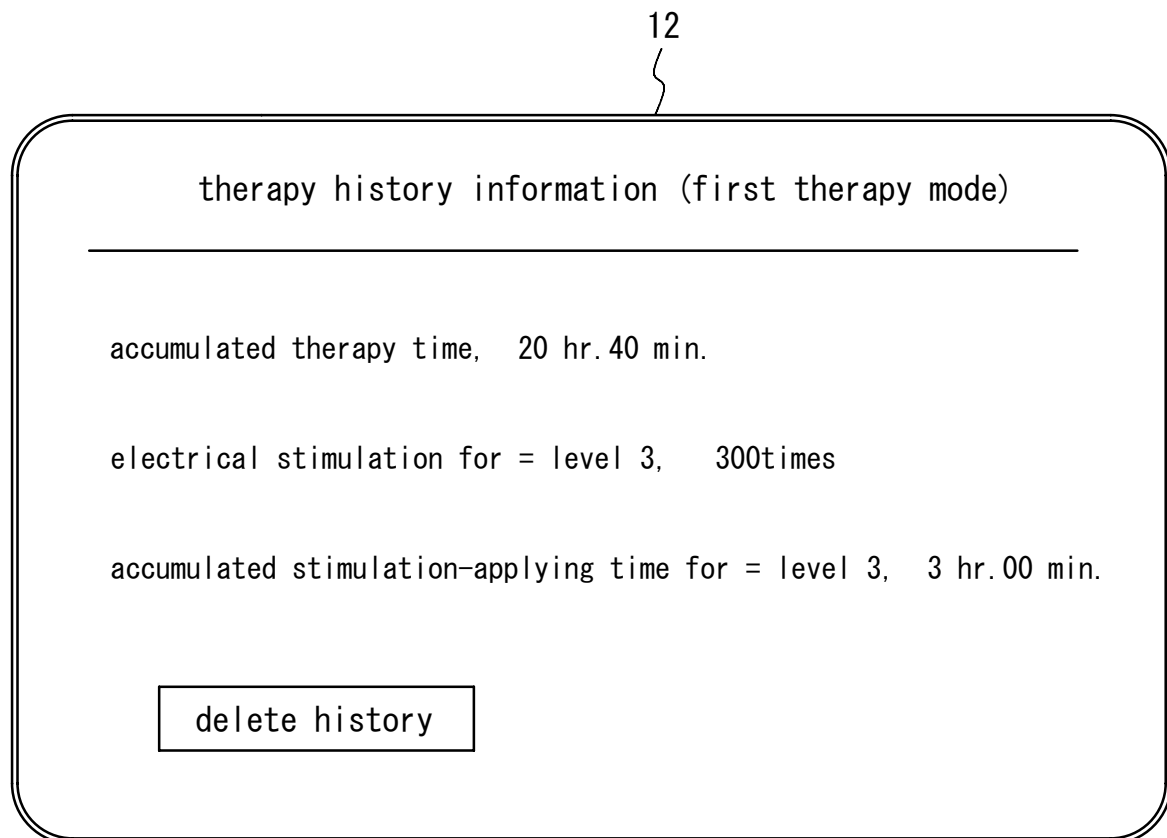


FIG. 10

