

FIG. 1

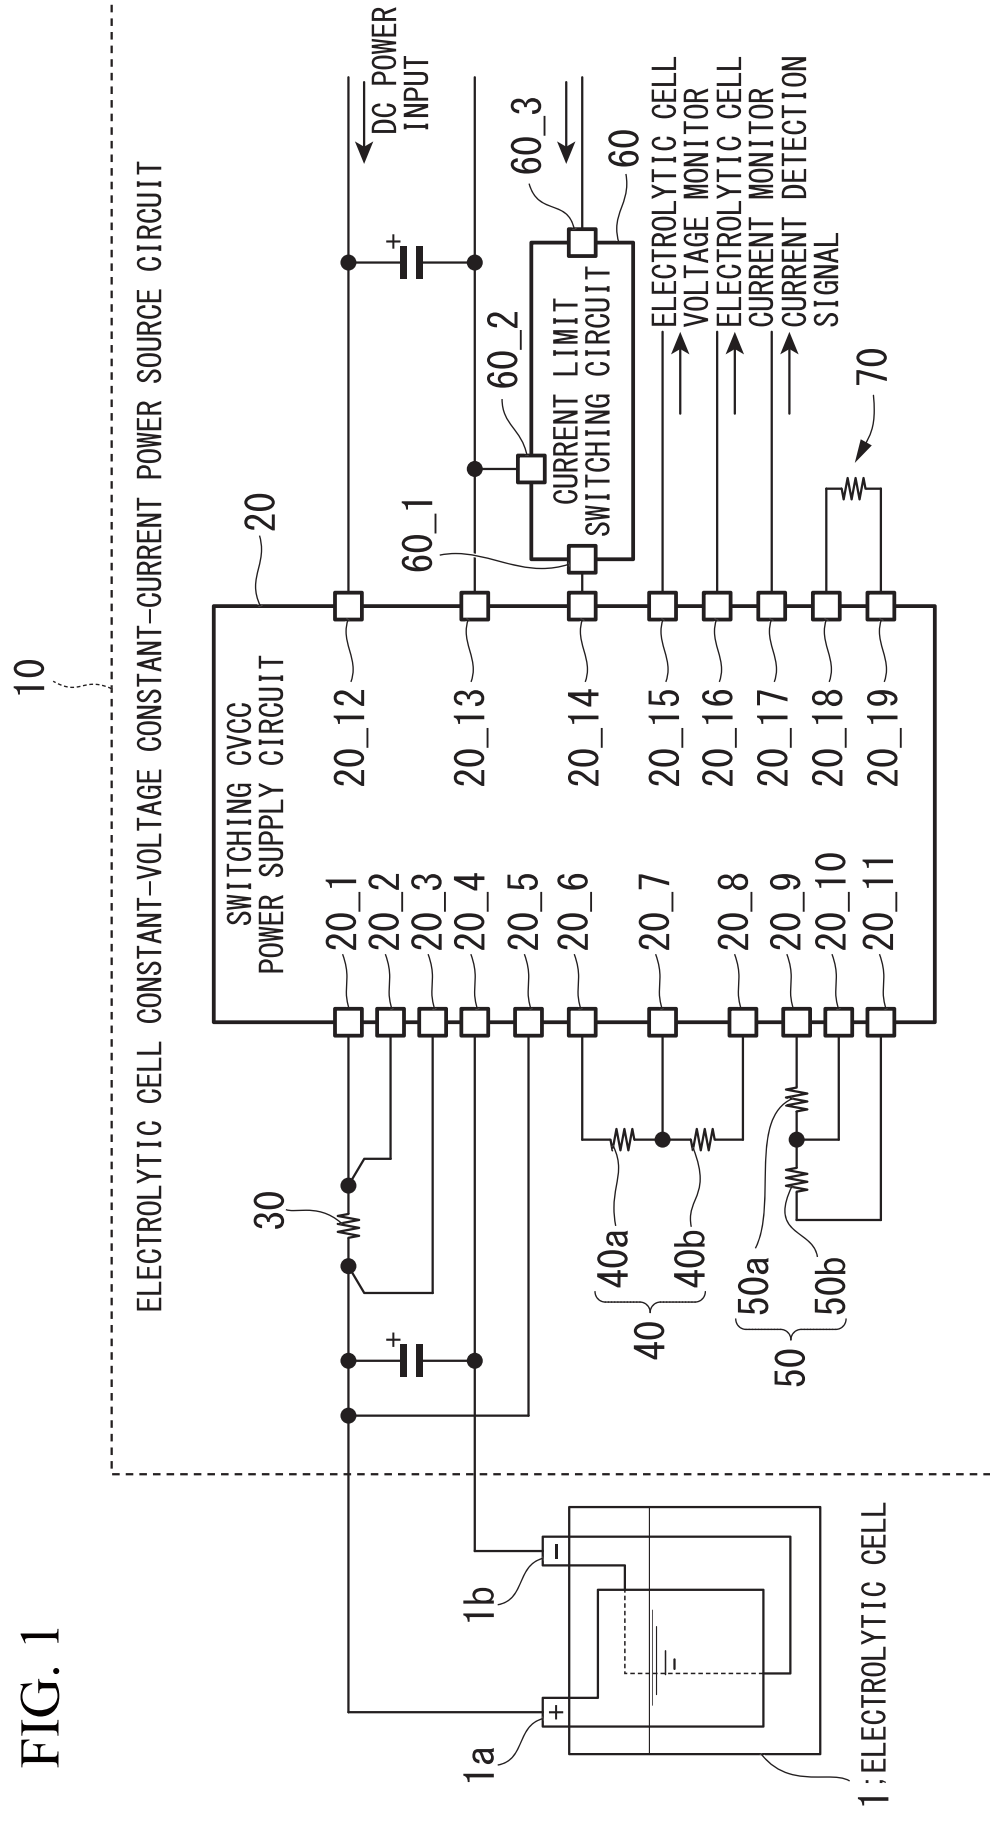


FIG. 2

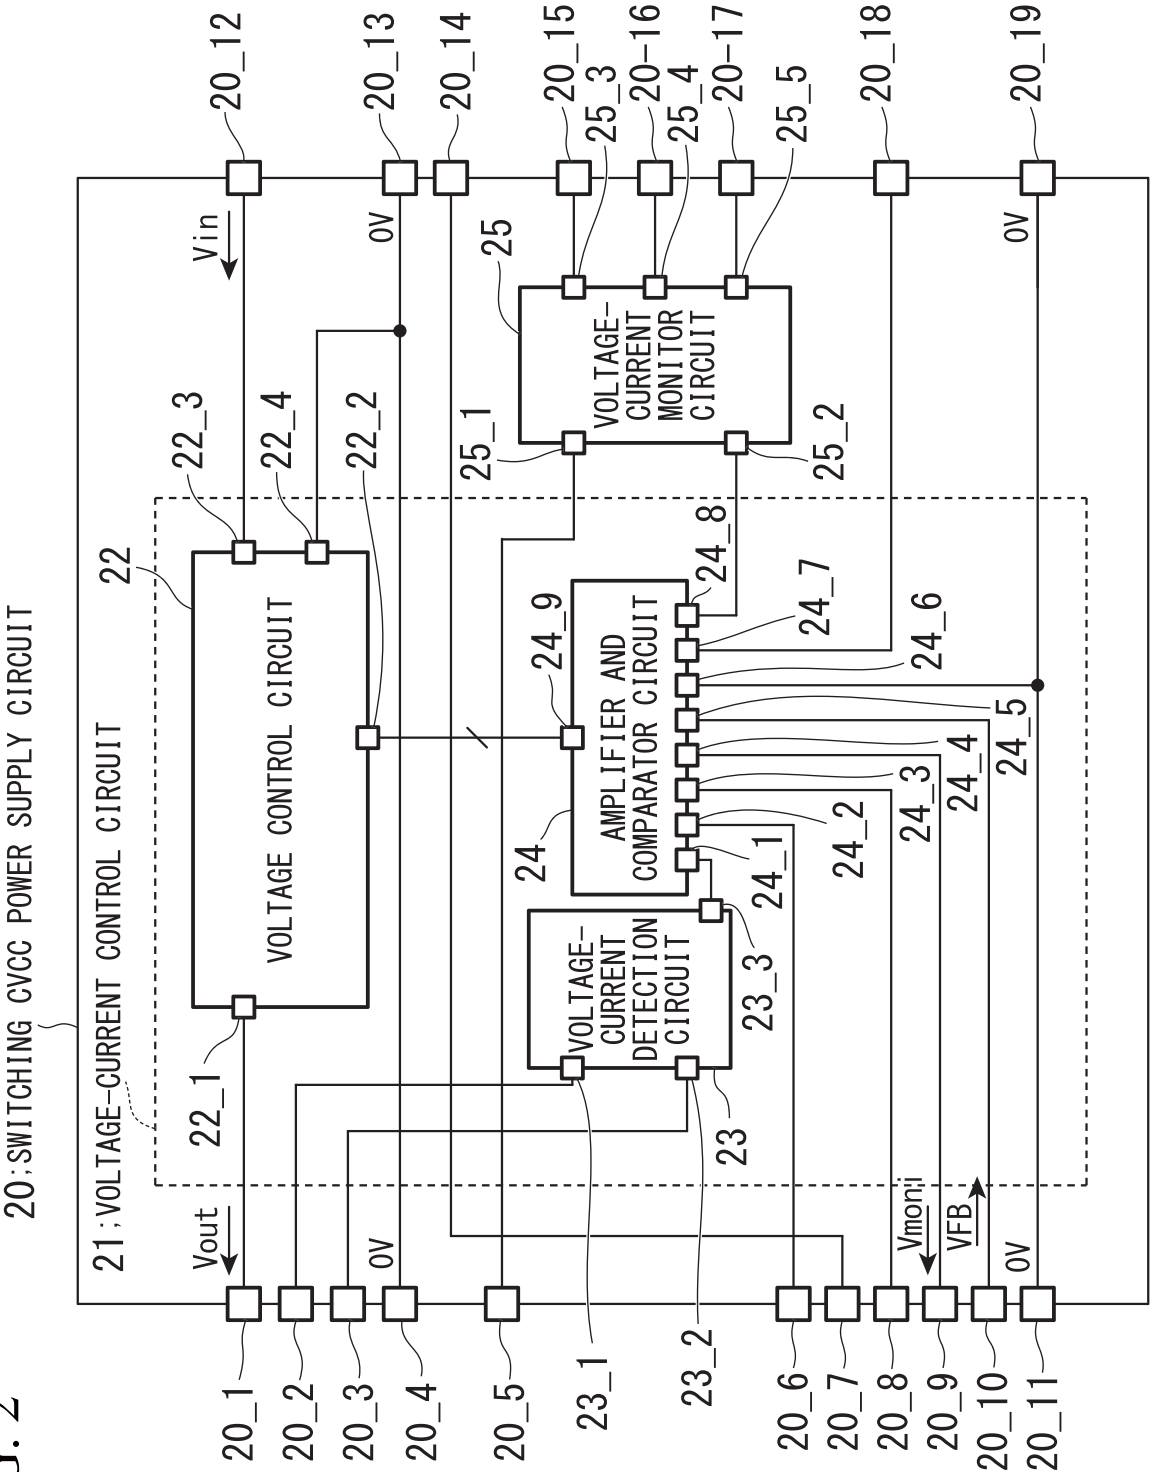


FIG. 3

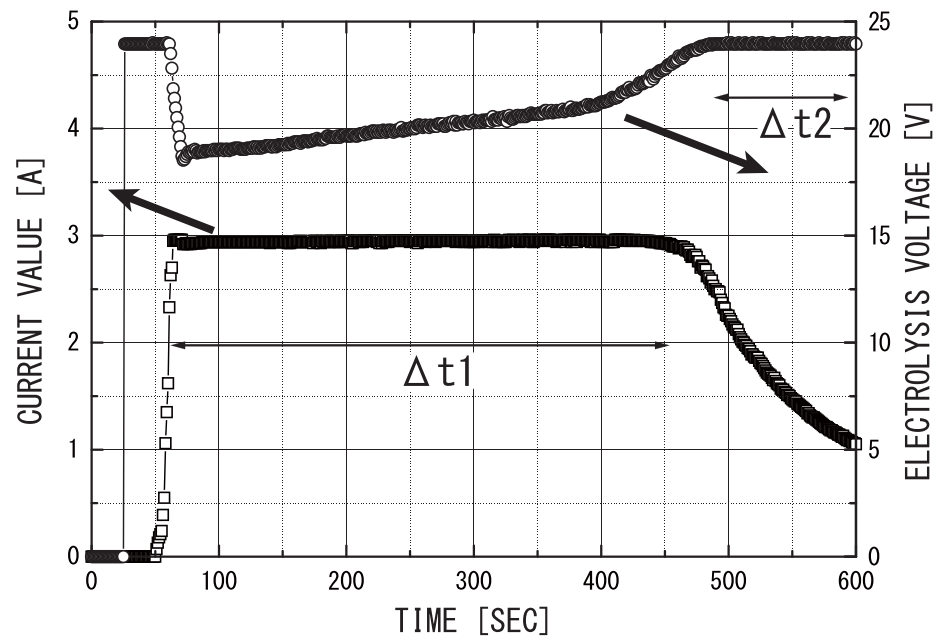


FIG. 4

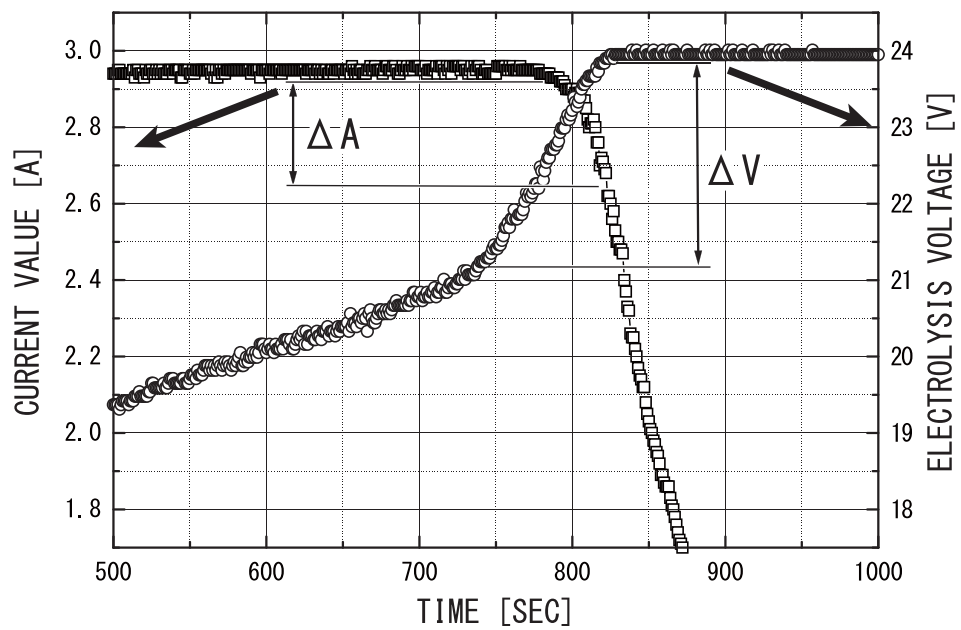


FIG. 5

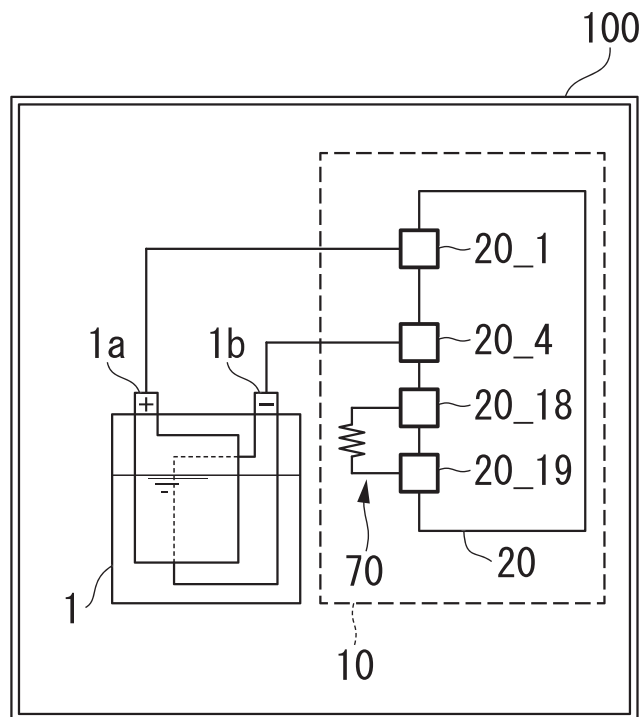


FIG. 6

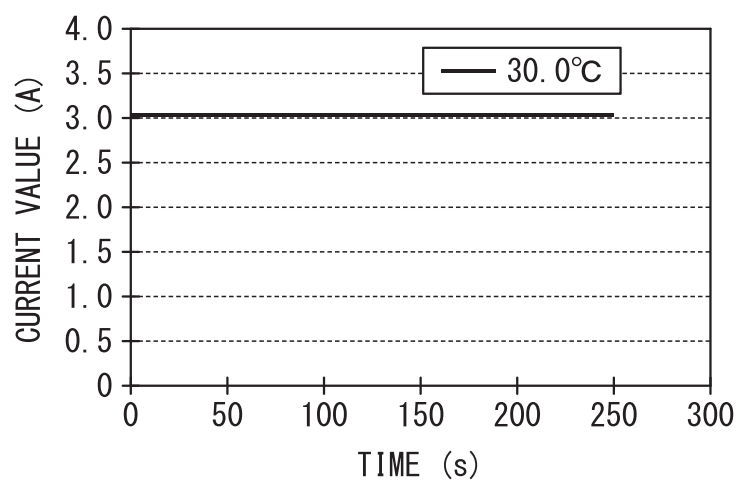


FIG. 7

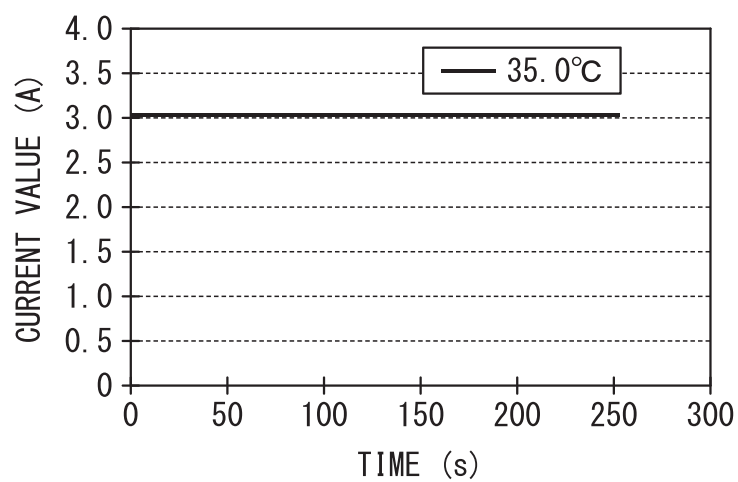


FIG. 8

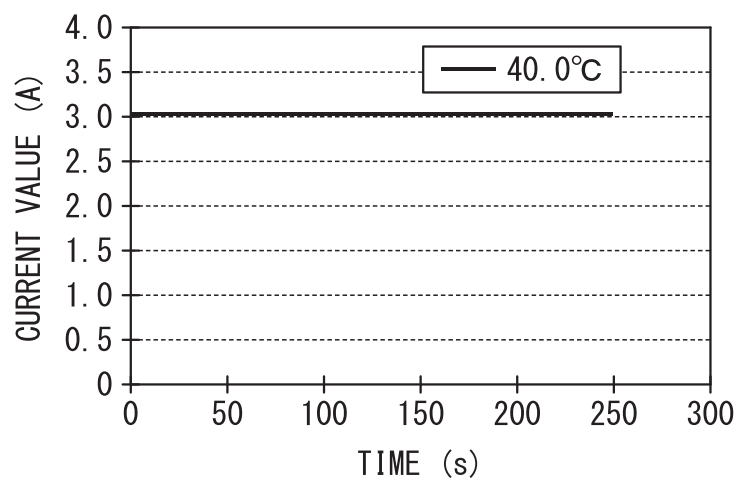


FIG. 9

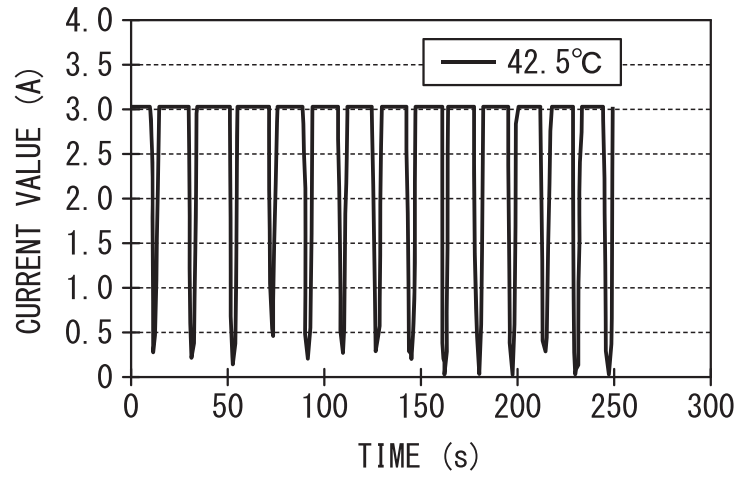


FIG. 10

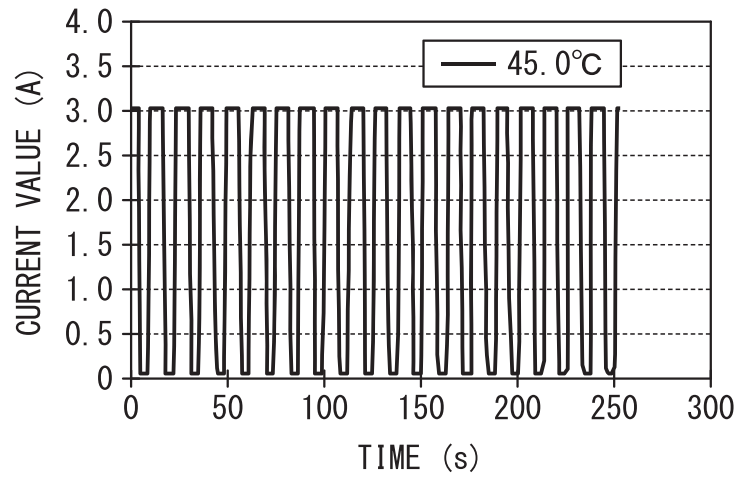


FIG. 11

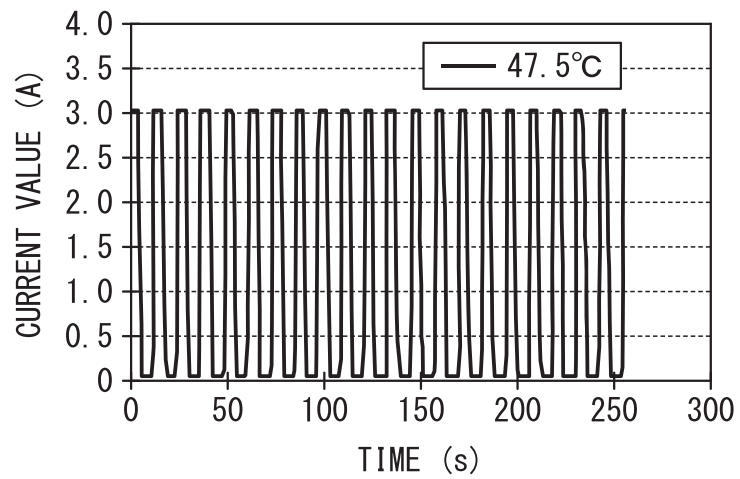


FIG. 12

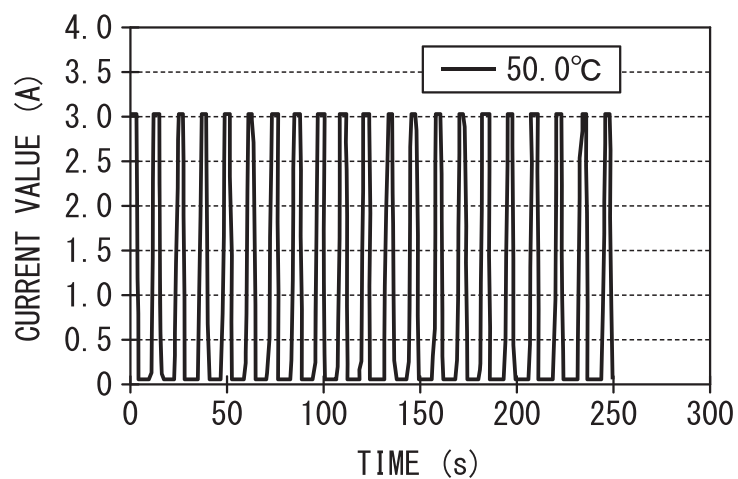


FIG. 13

ENVIRONMENTAL TEMPERATURE (° C)	AVERAGE CURRENT VALUE (A)	EFFECTIVE CHLORINE CONCENTRATION (ppm)	ELECTROLYTIC CELL TEMPERATURE (° C)
30.0	3.0	20	41.3
35.0	3.0	21	45.8
40.0	3.0	17	46.6
42.5	2.5	13	47.7
45.0	1.8	6	46.2
47.5	1.3	3	49.1
50.0	1.0	1	49.2

FIG. 14

