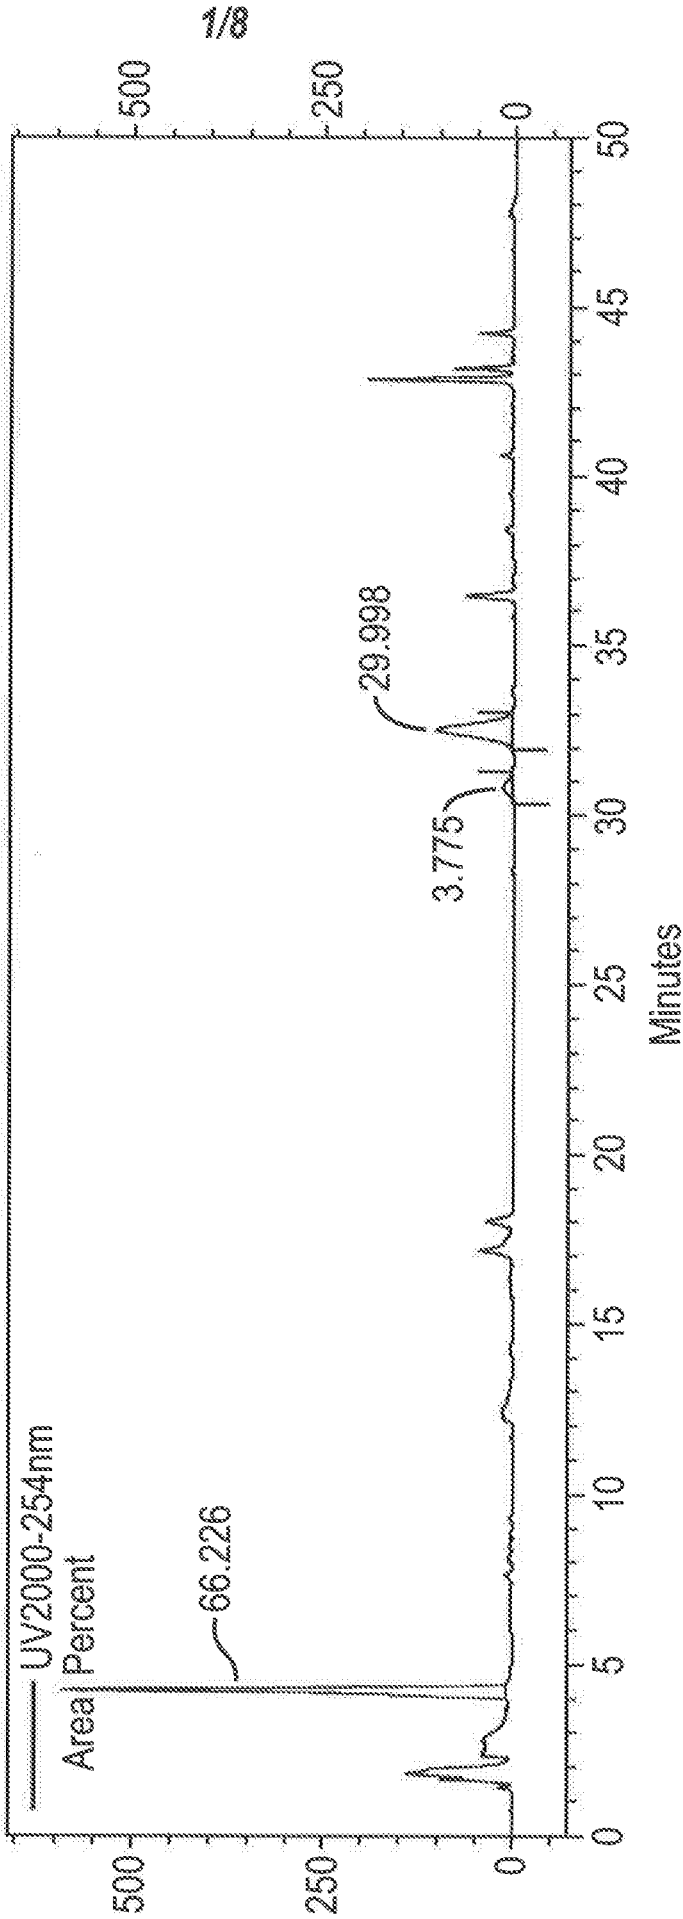


FIG. 1



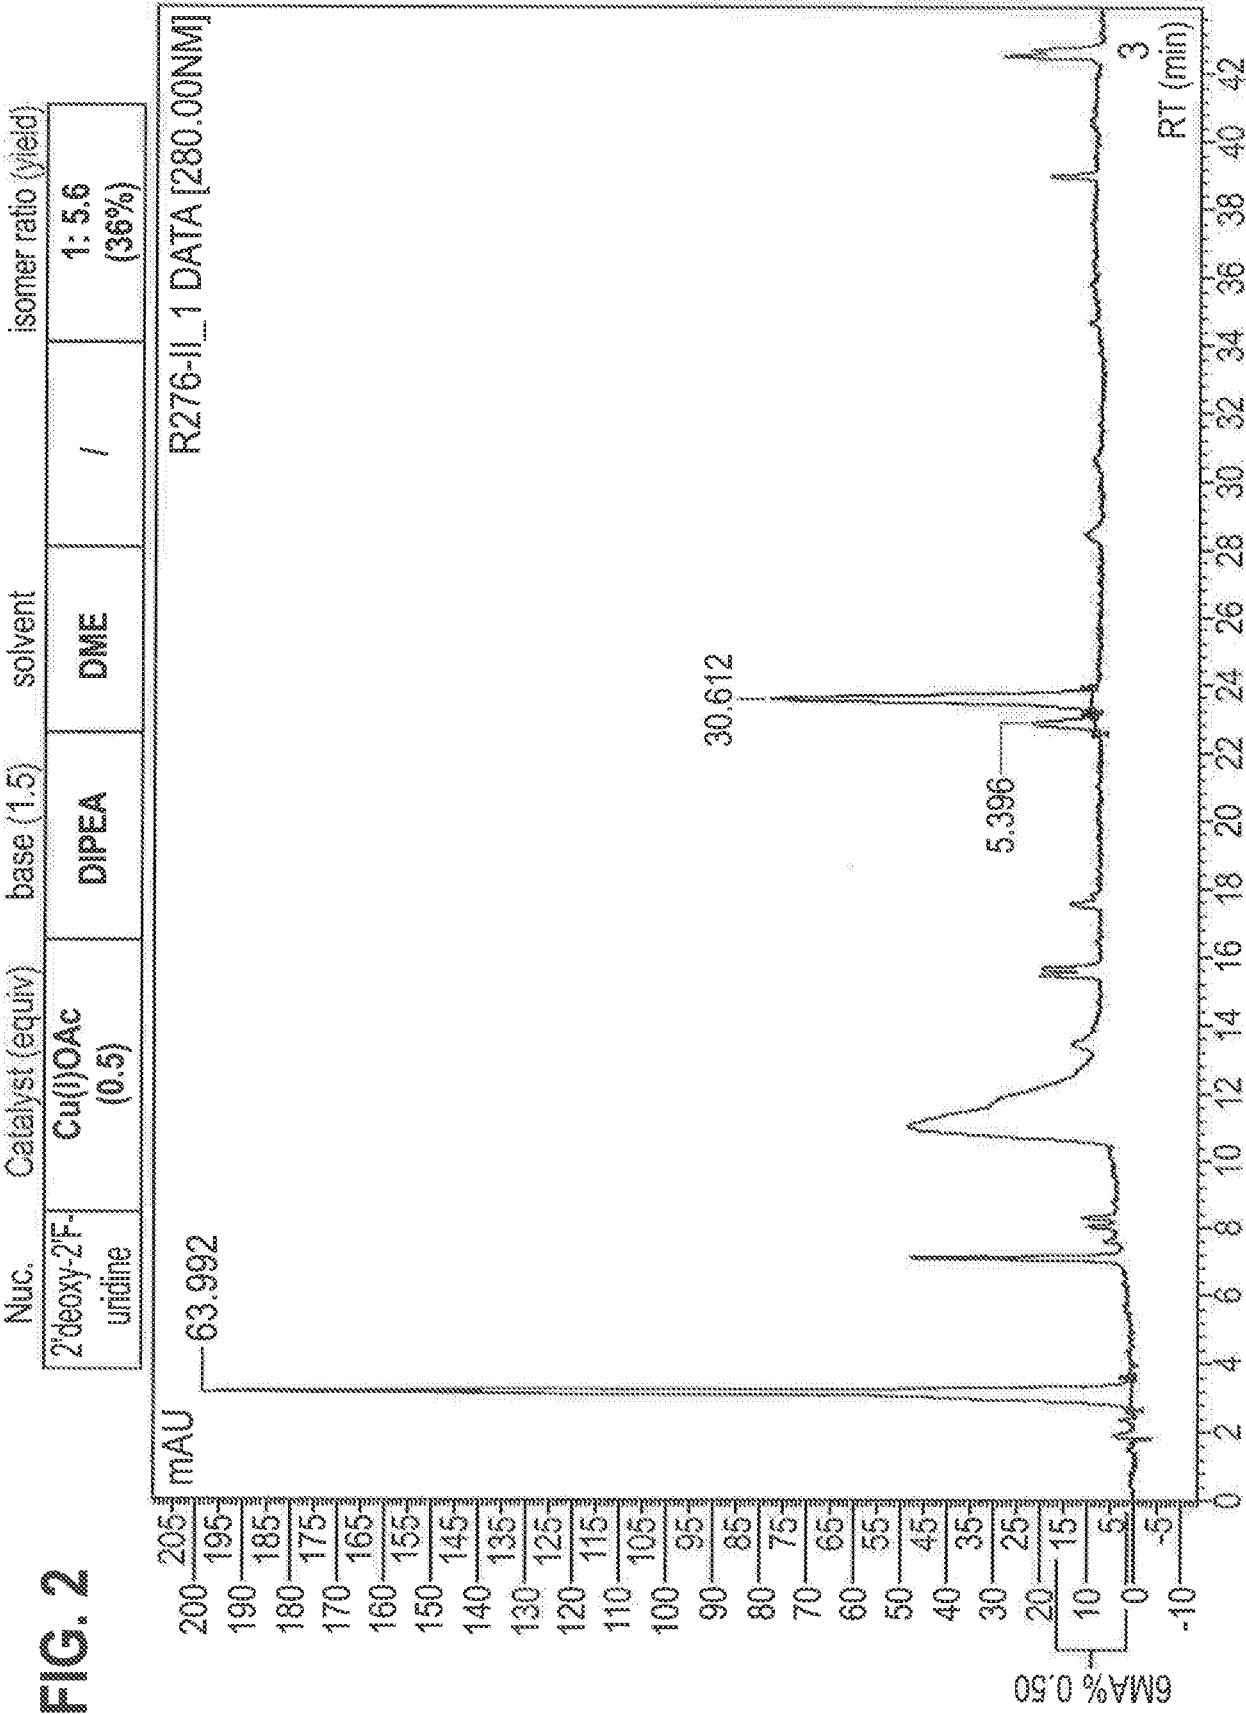


FIG. 3




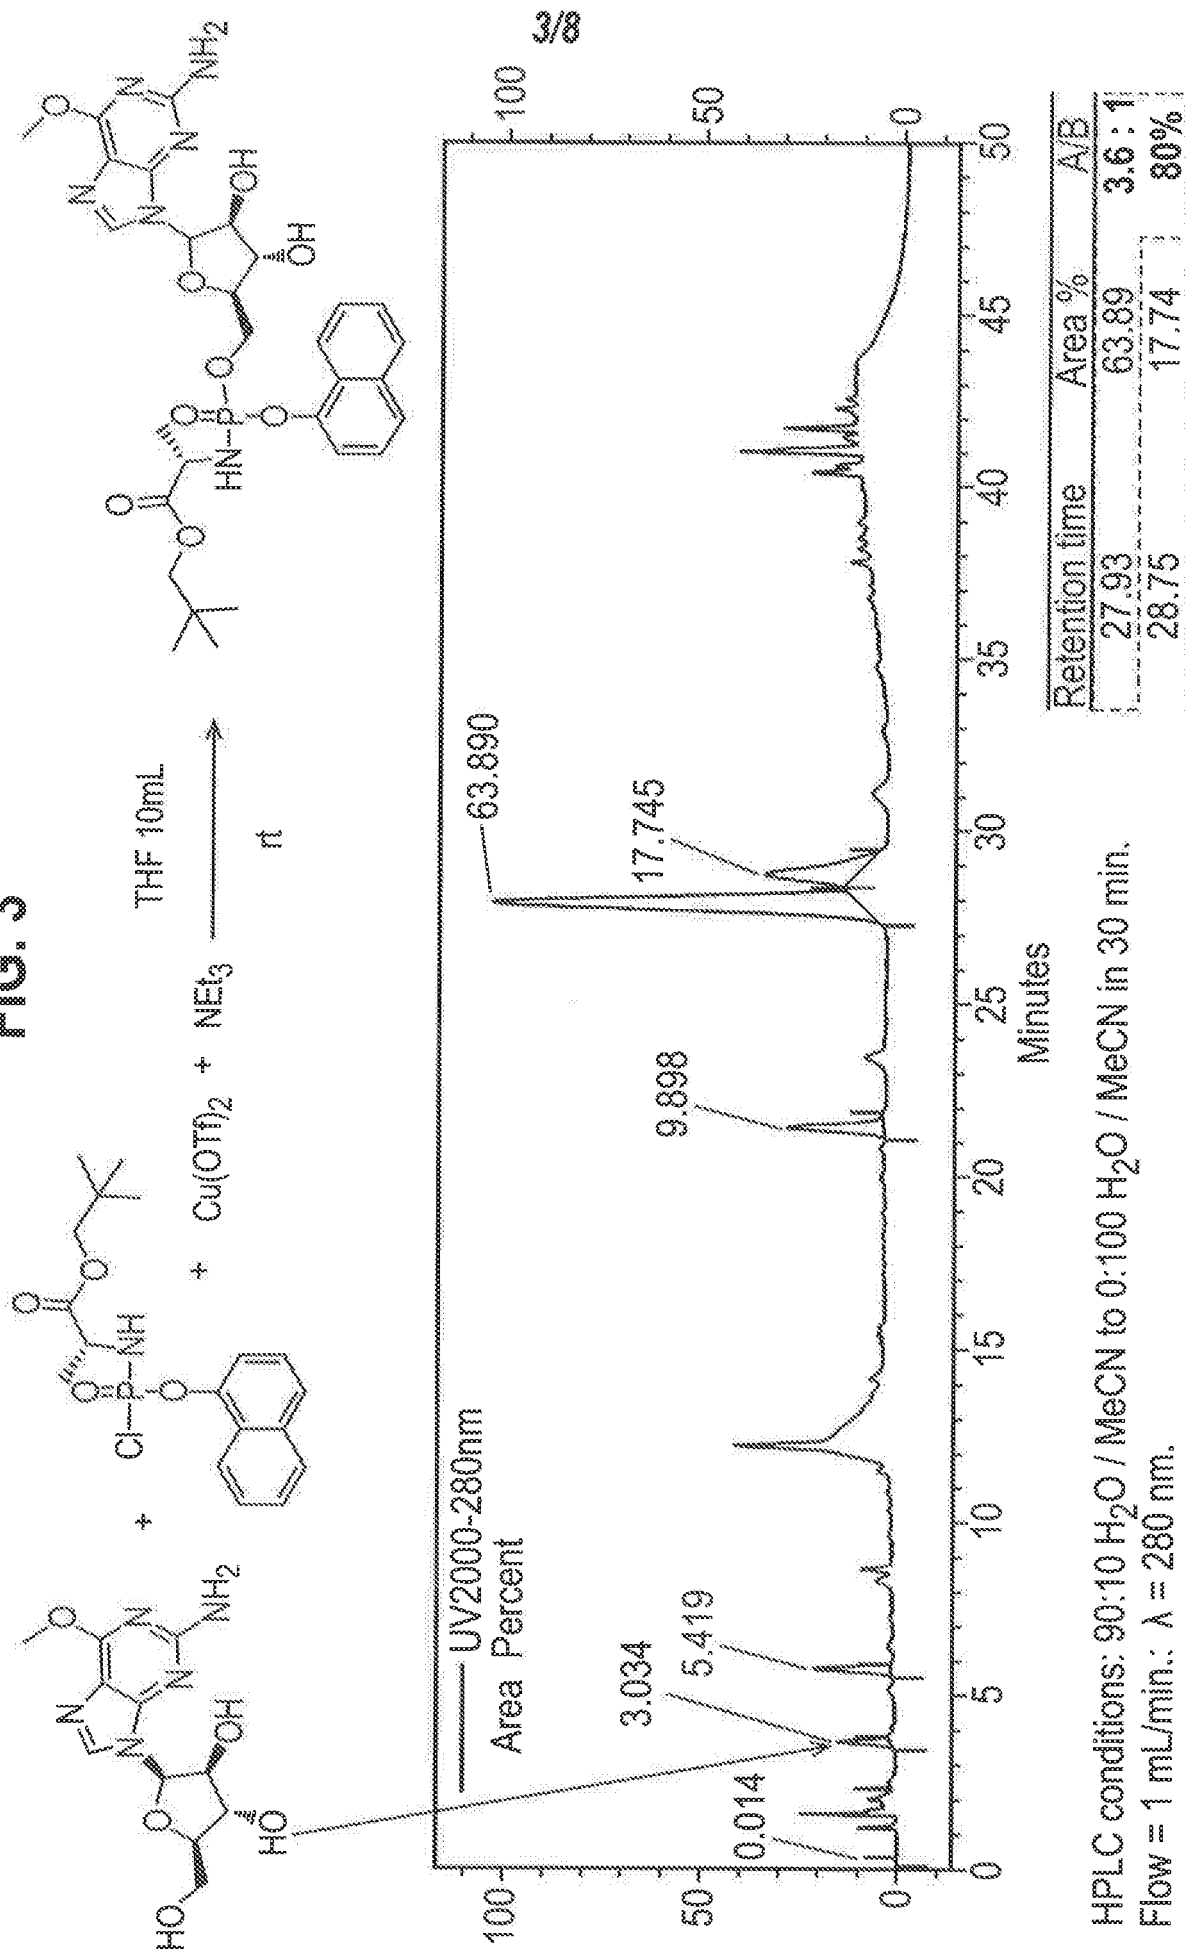


FIG. 4

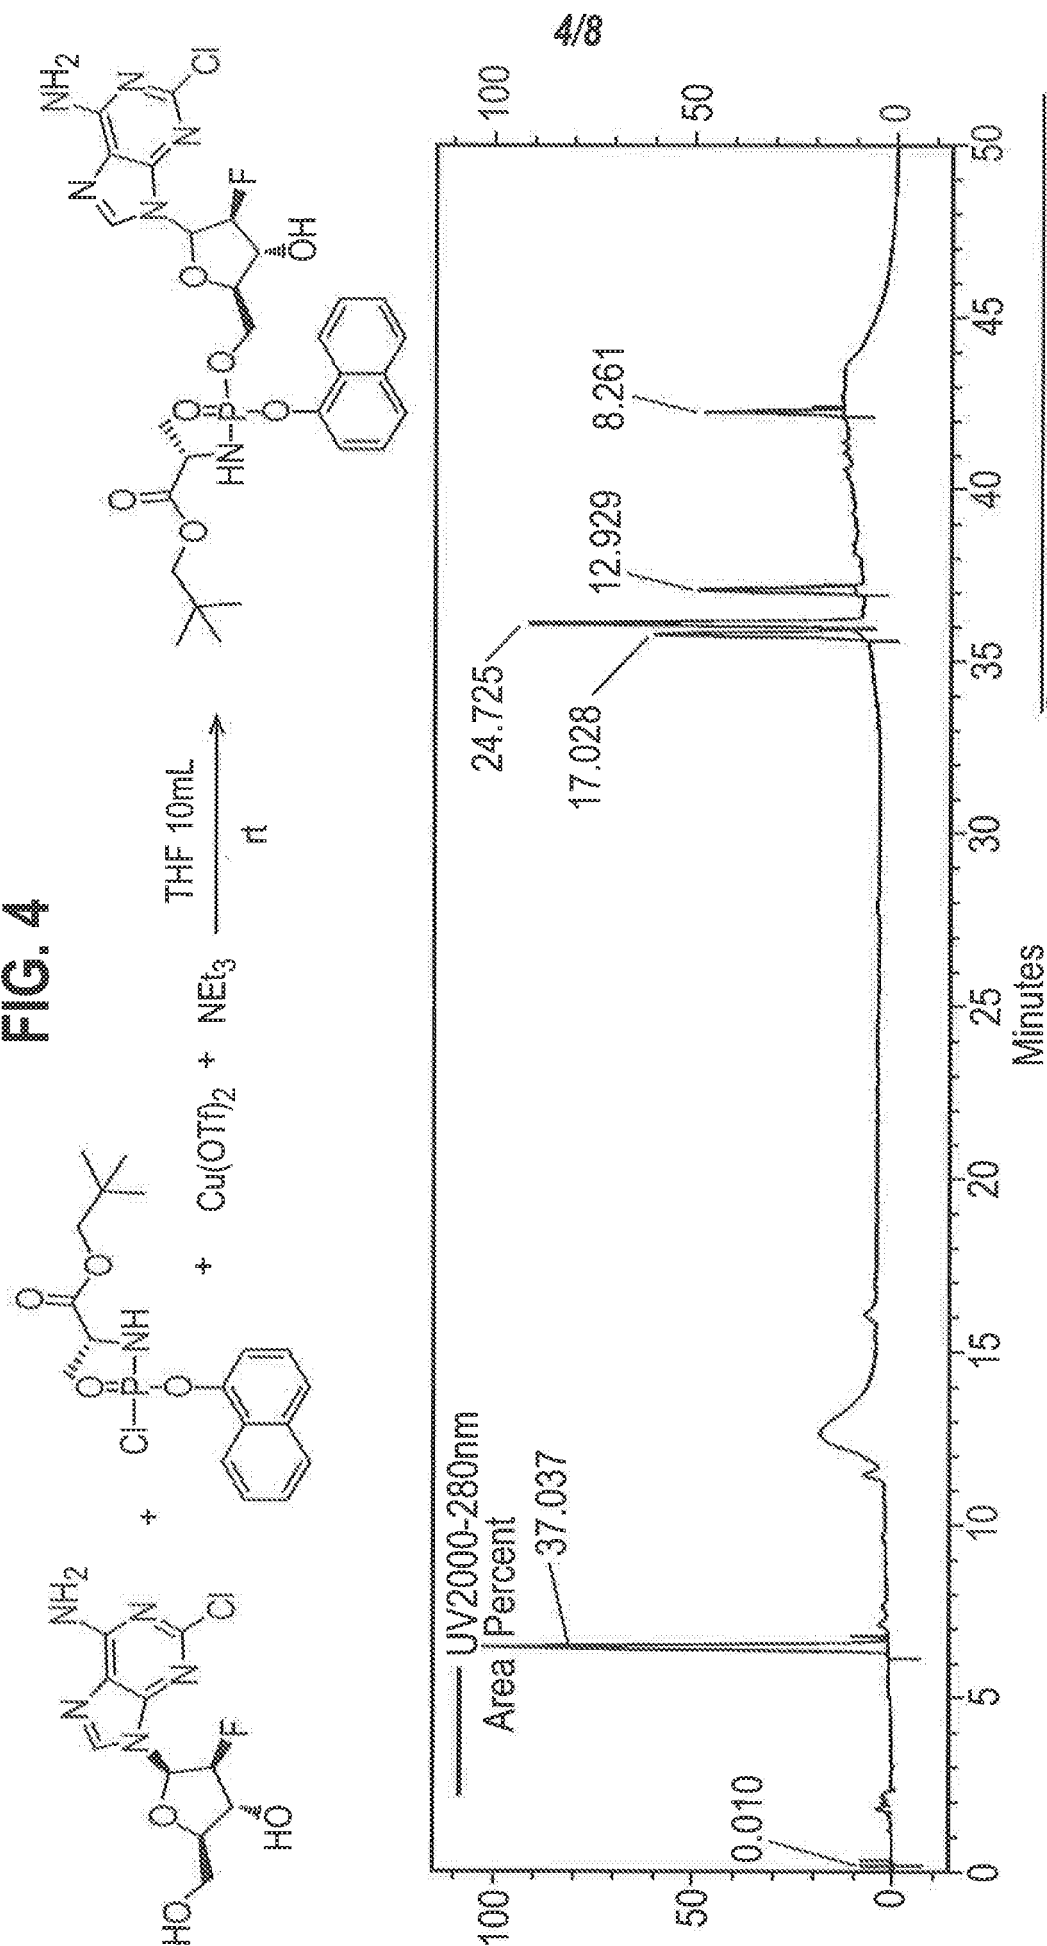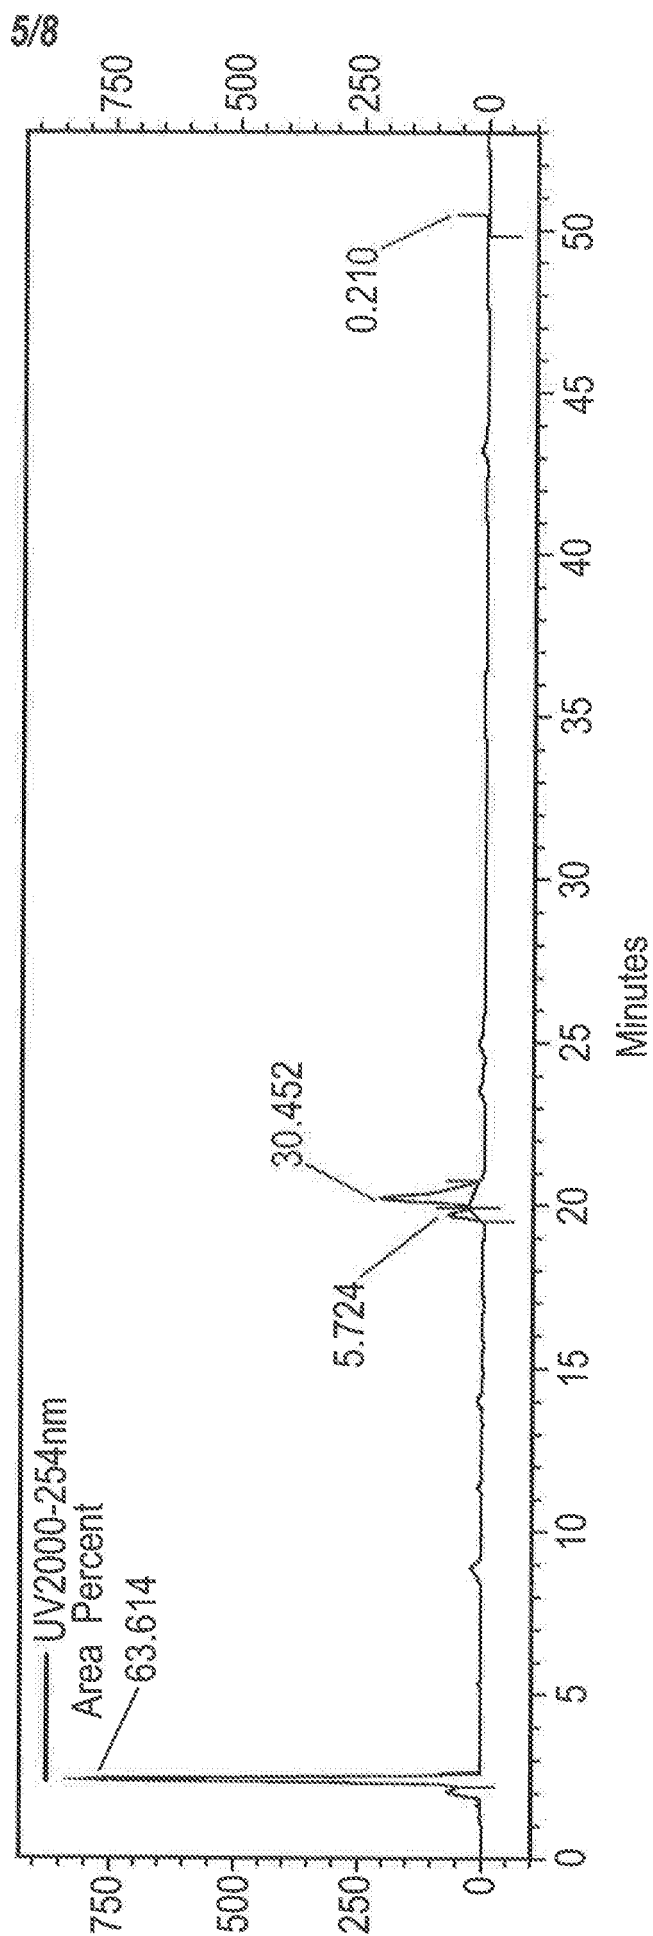

HPLC conditions: 90:10 H_2O / MeCN to 0:100 H_2O / MeCN in 30 min.
Flow = 1 mL/min.; λ = 254 and 280 nm.

FIG. 5

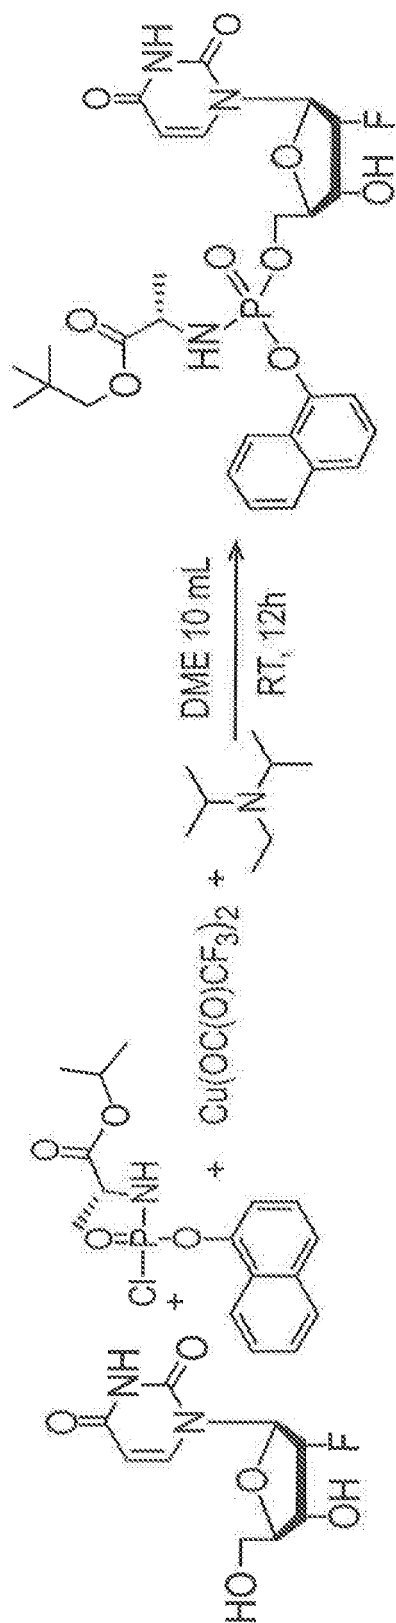

6/8

FIG. 6

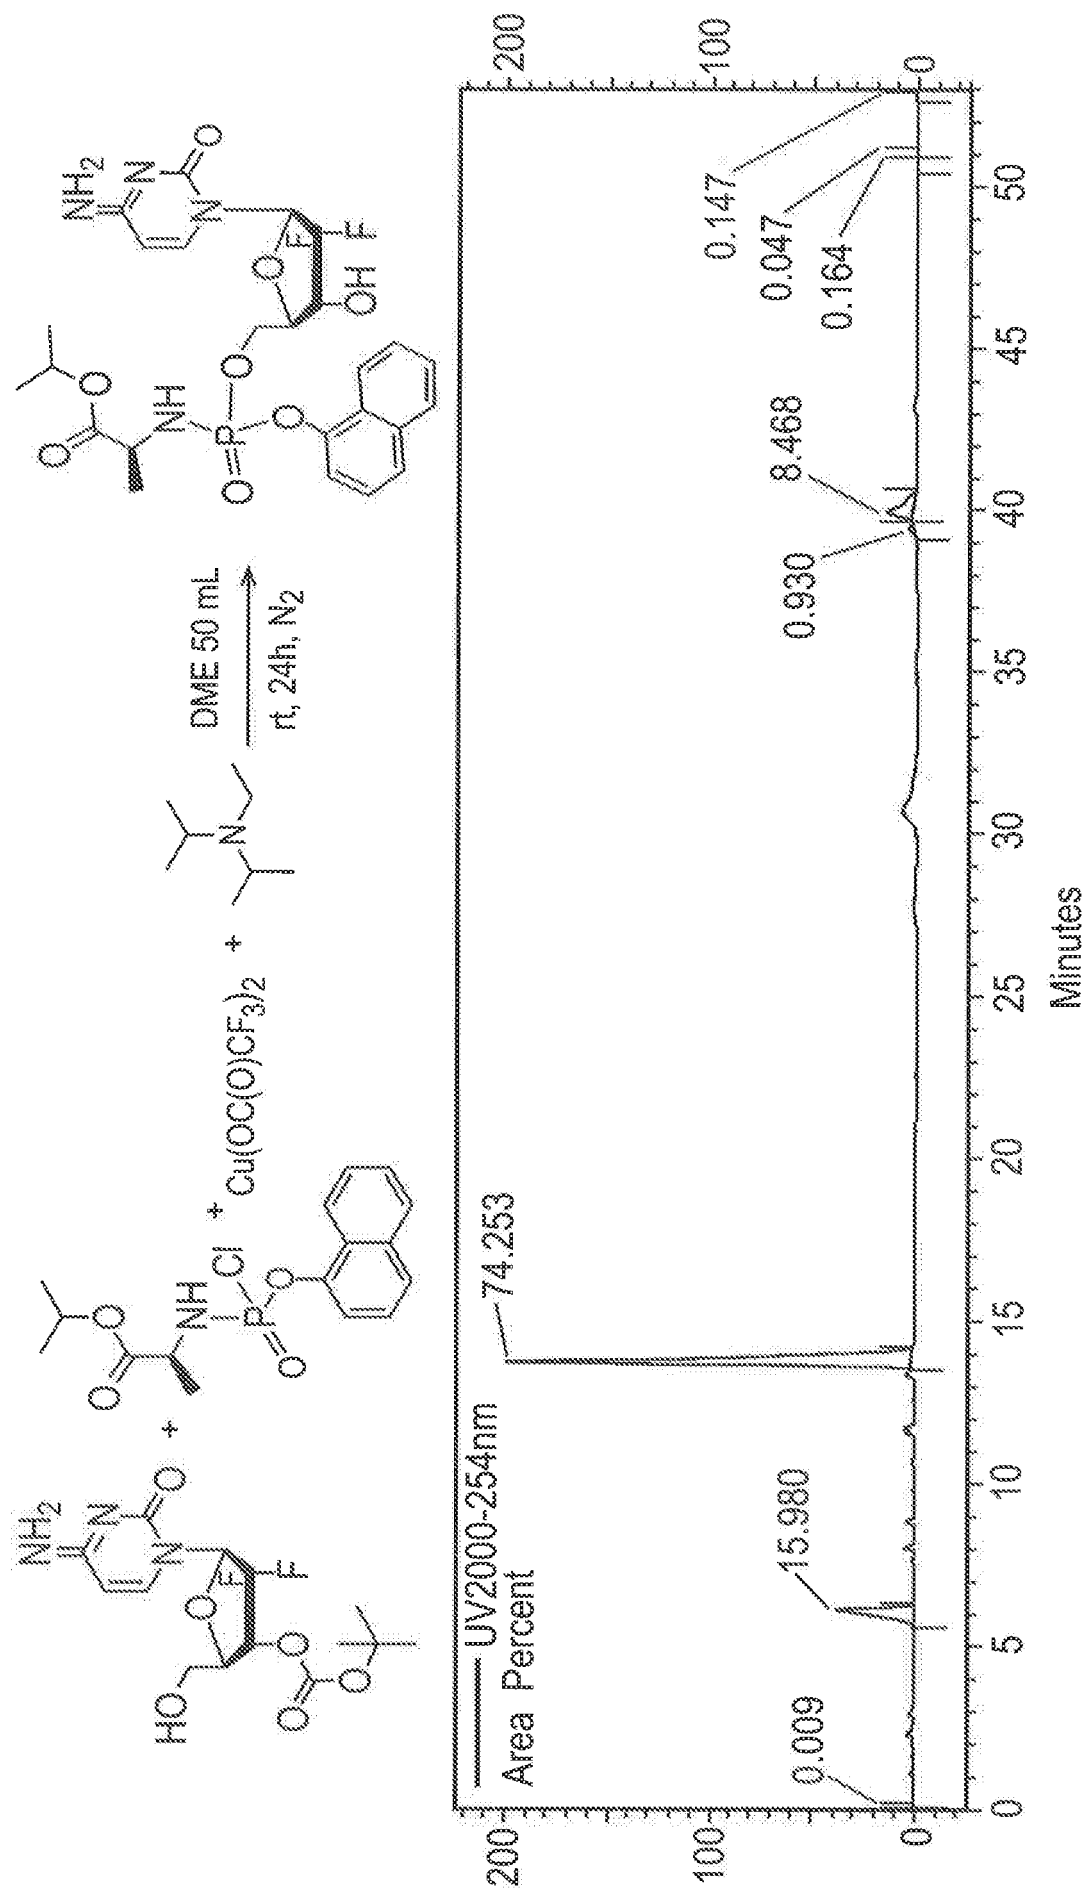


FIG. 7

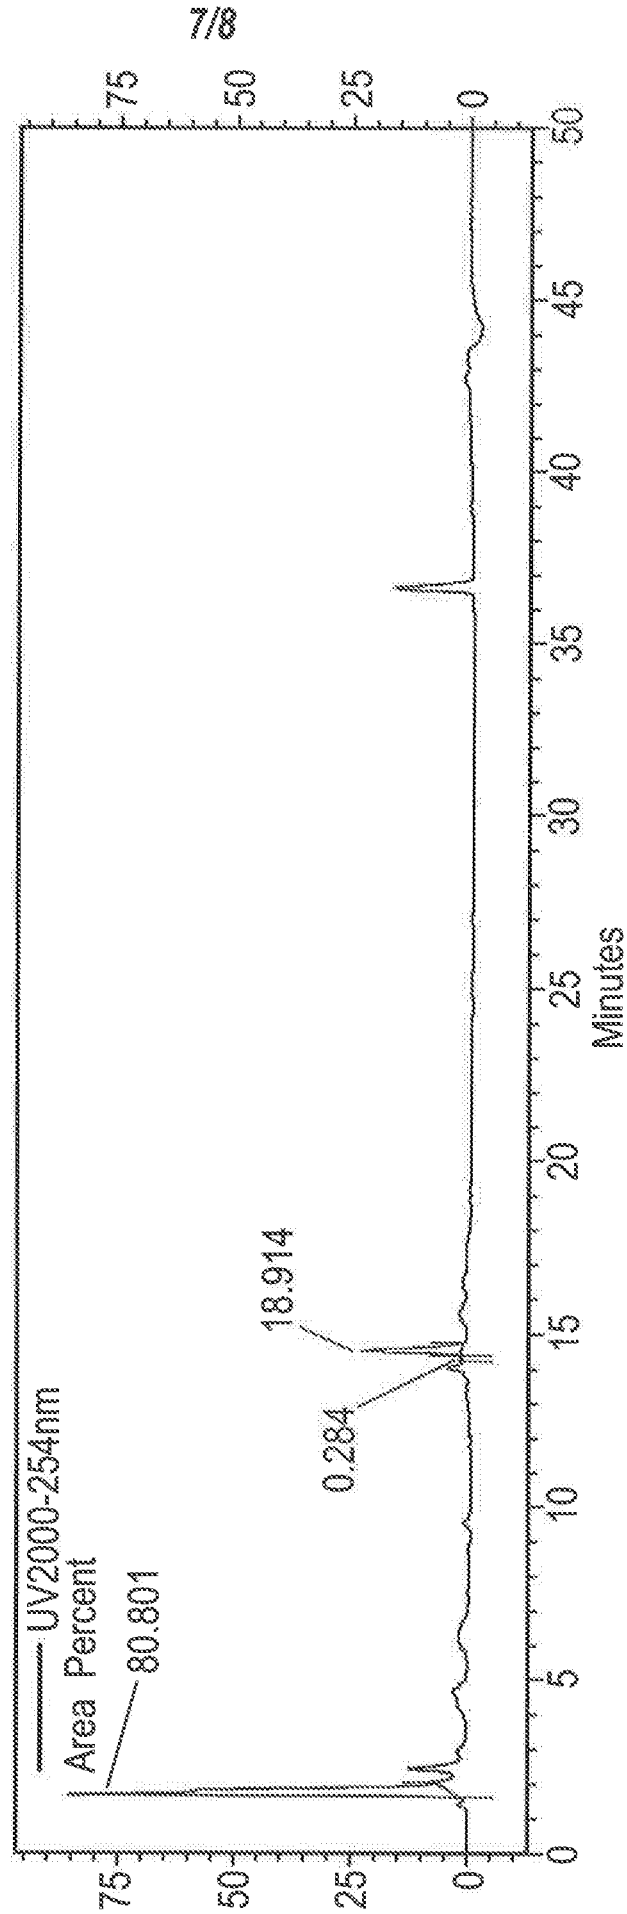


FIG. 8

