




[図1]

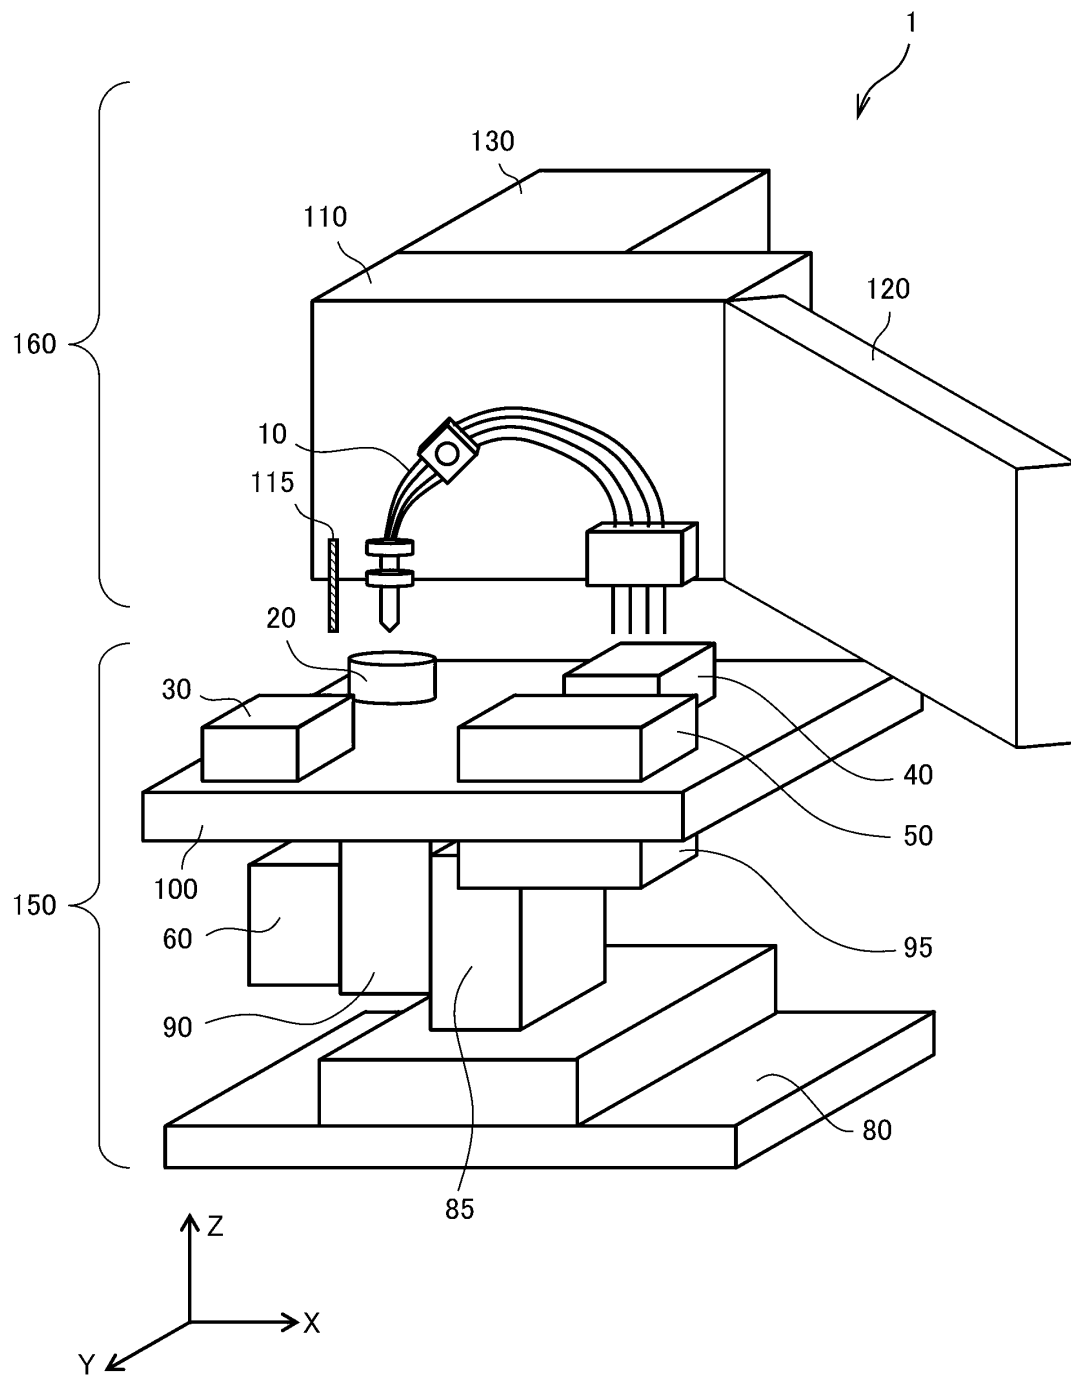


[図2]

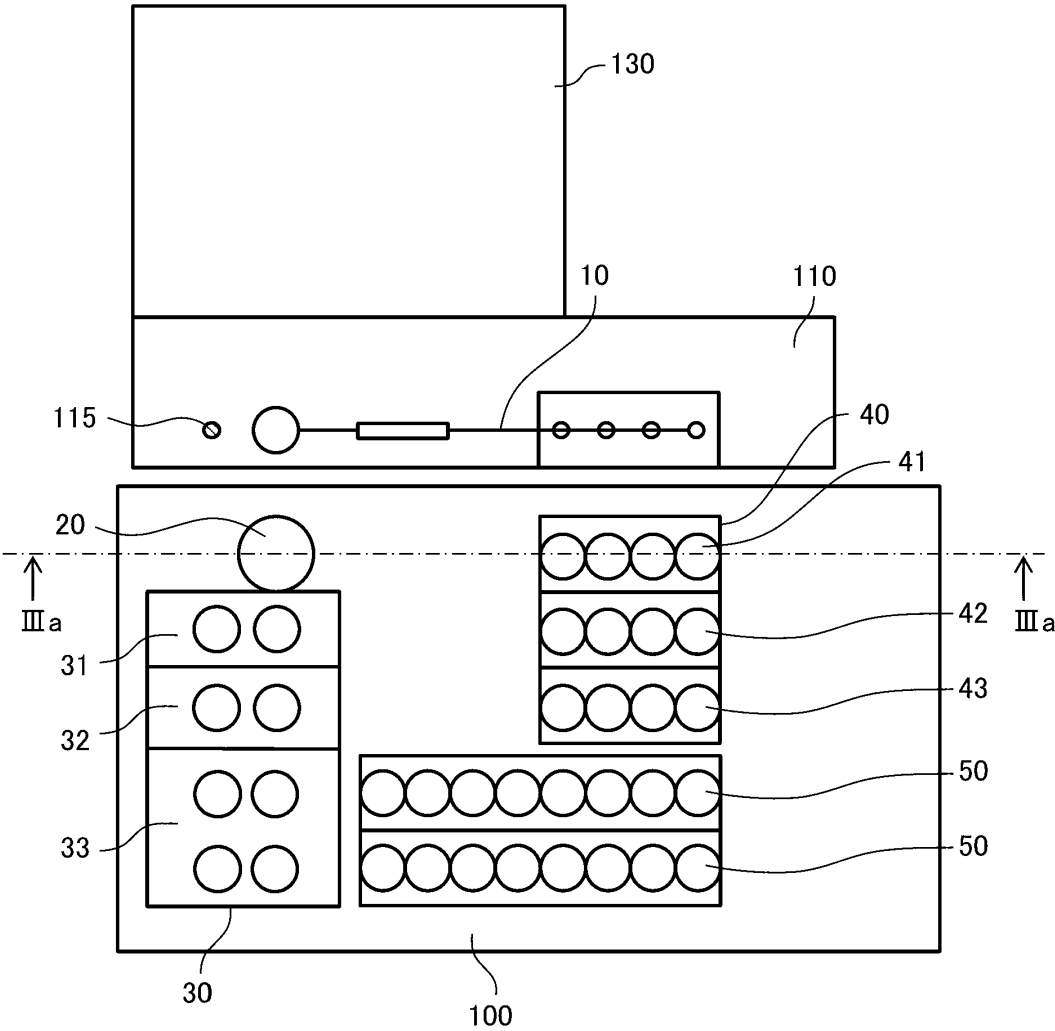


[図3A]

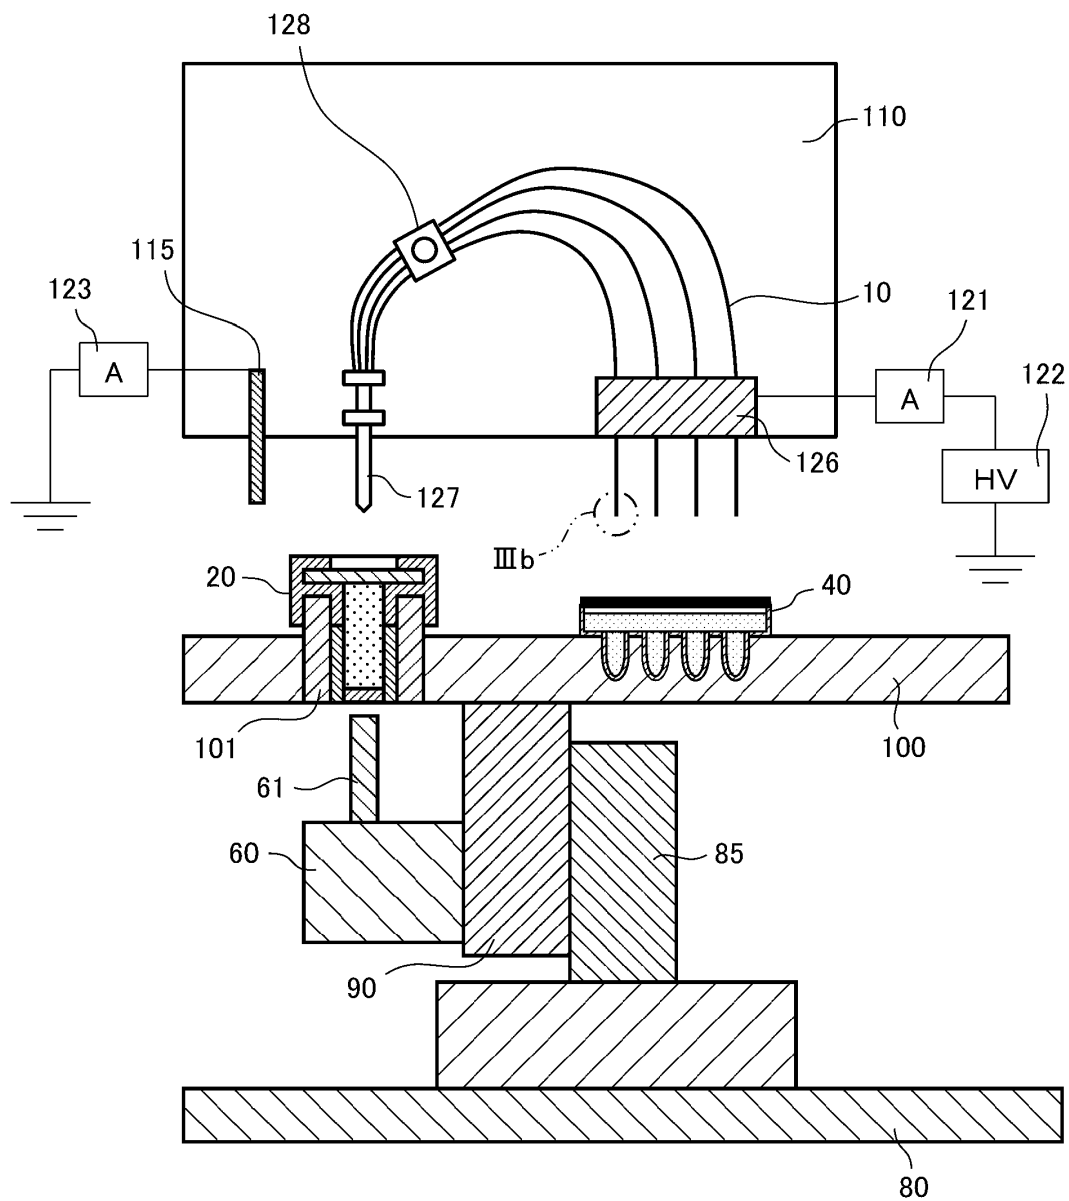


[図3B]

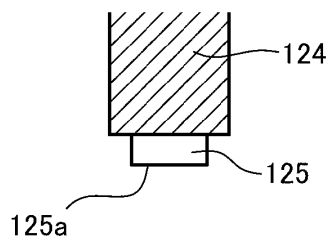

[図4]

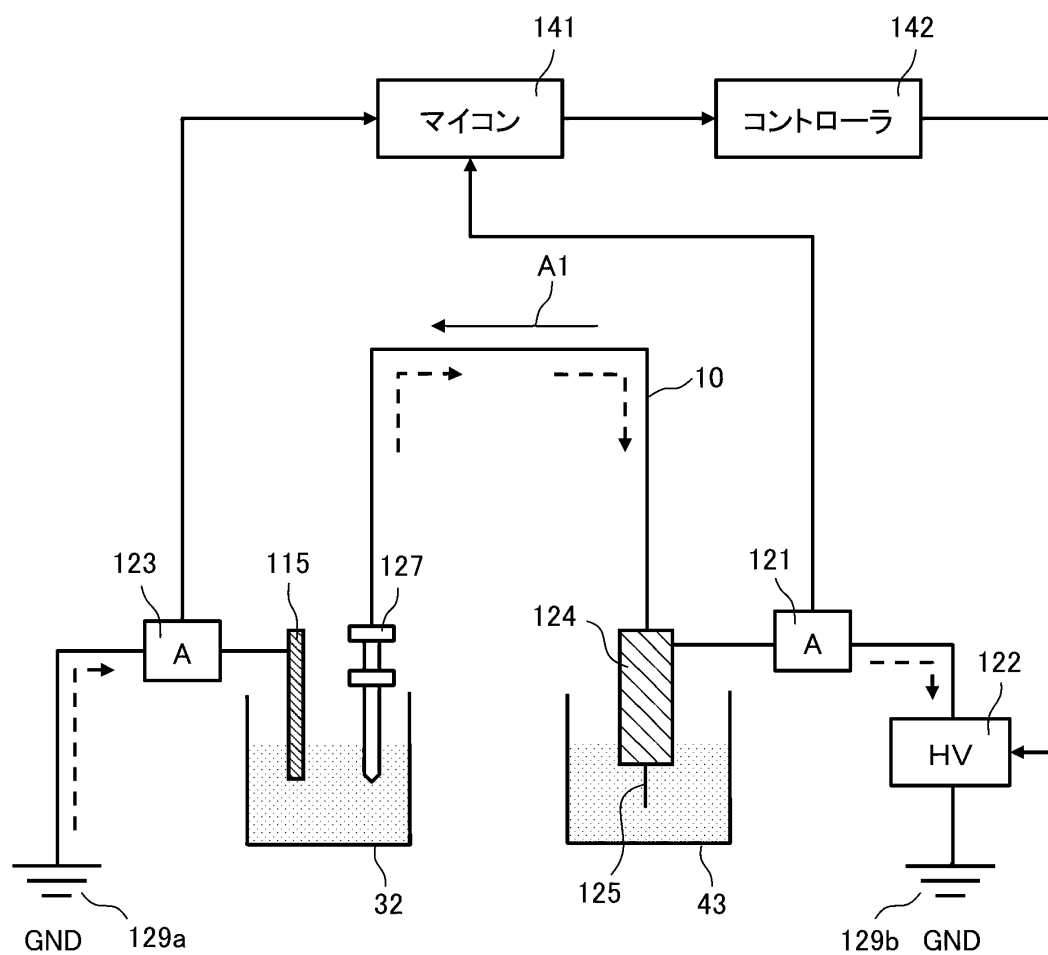

[図5]

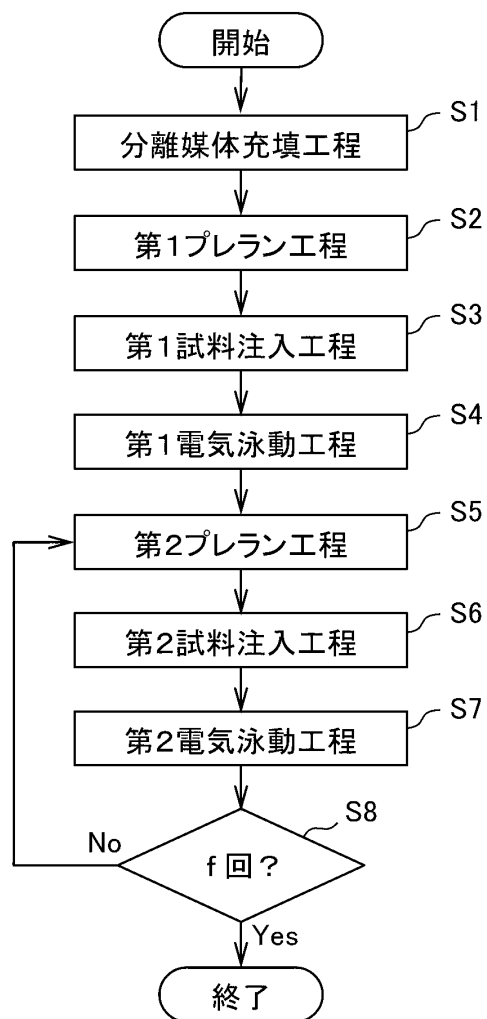


[図6]


Setup Strip Information > Edit Strip Information (A) > Select Assay (1st)

Assay	T_Seq_36_Fast	▽	
Application	Sequencing		
Polymer	Polymer7		
Dye Set	T 4-dye sequencing		
Instrument Protocol	Fast_Sequence36_Polymer7		Details
Analysis Protocol	Basecalling_T_FastSeq		Details
Polymer exchange frequency	every 4 injection		
☐ Cancel		Clear	 Apply


[図7]

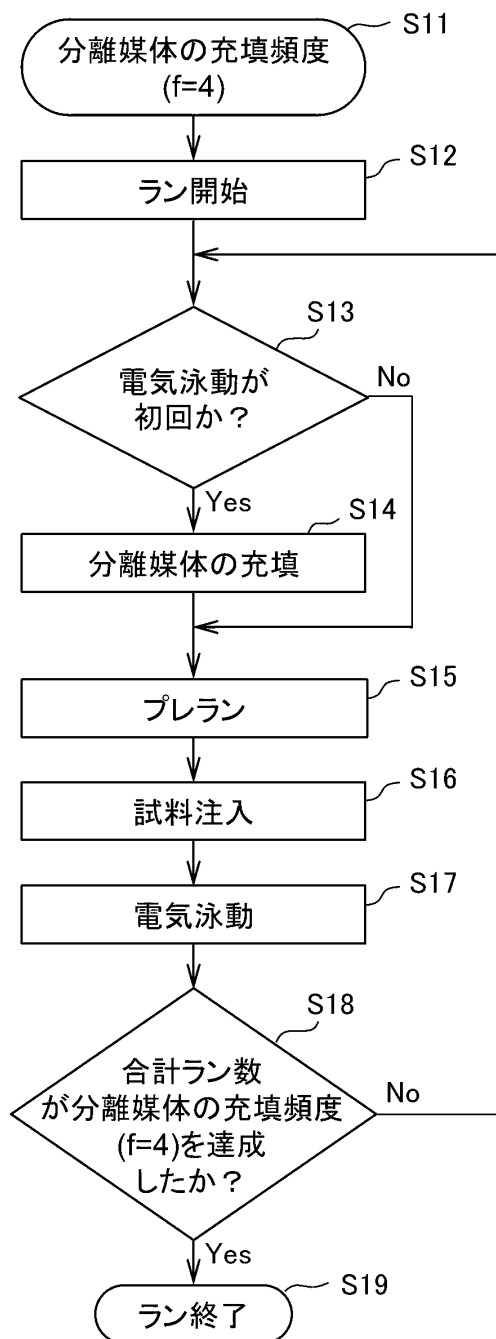


[図8]

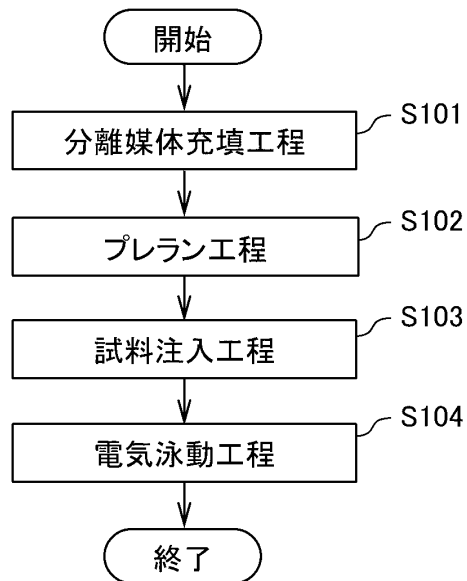

[図9]

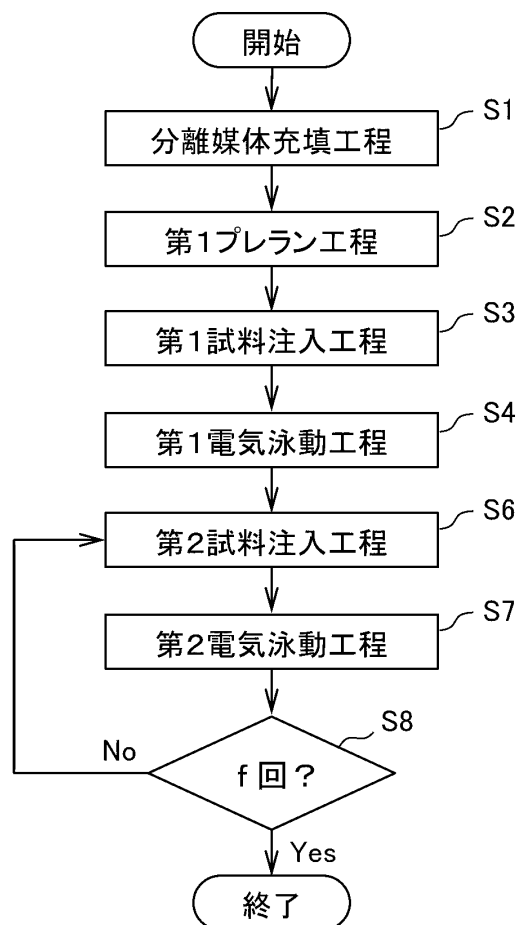


[図10]

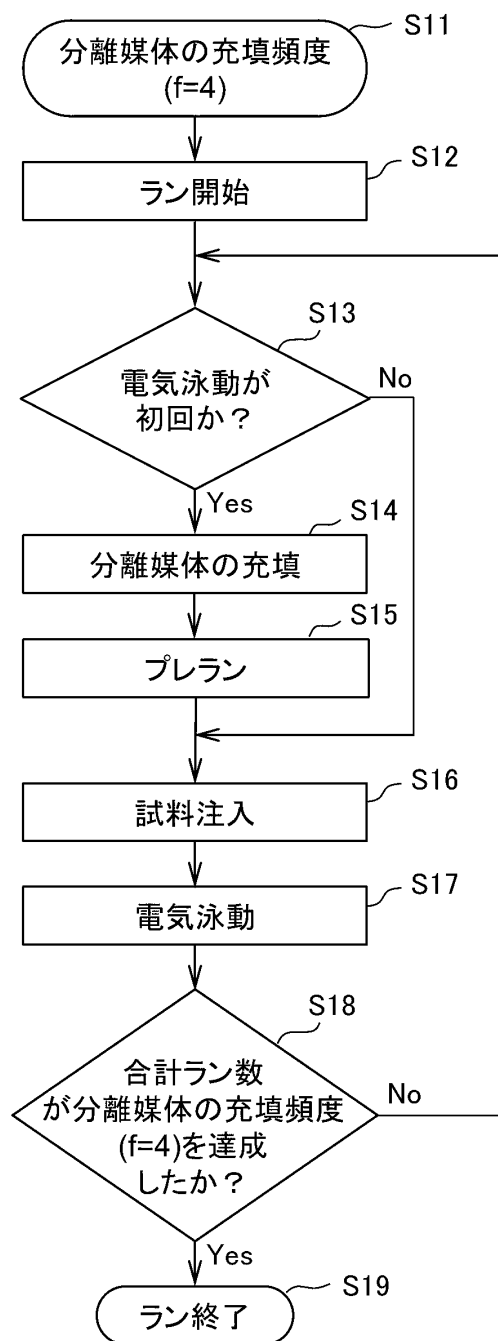


[図11]


400 bp付近

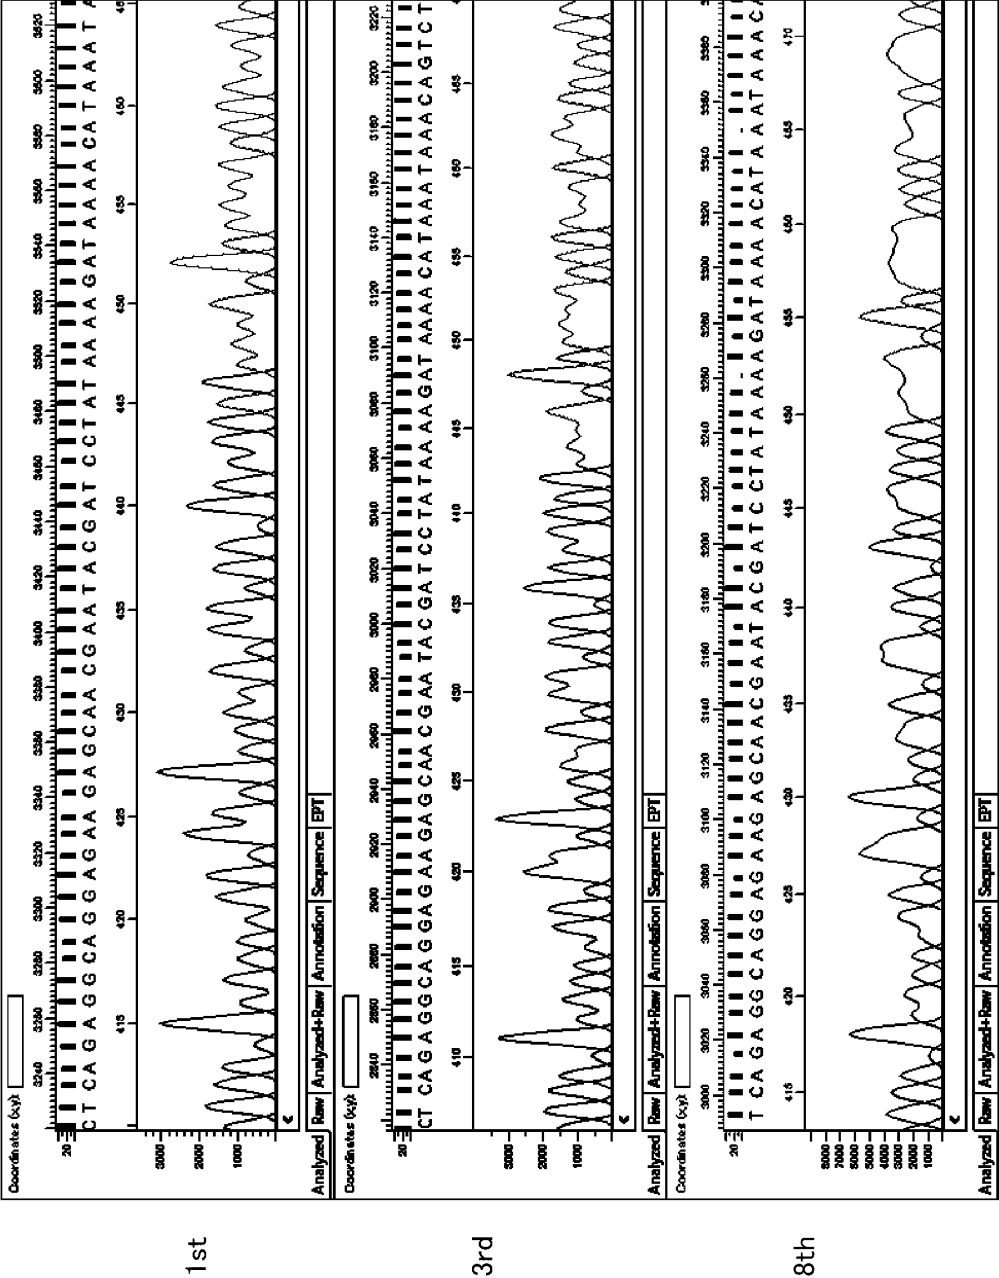


[図12]

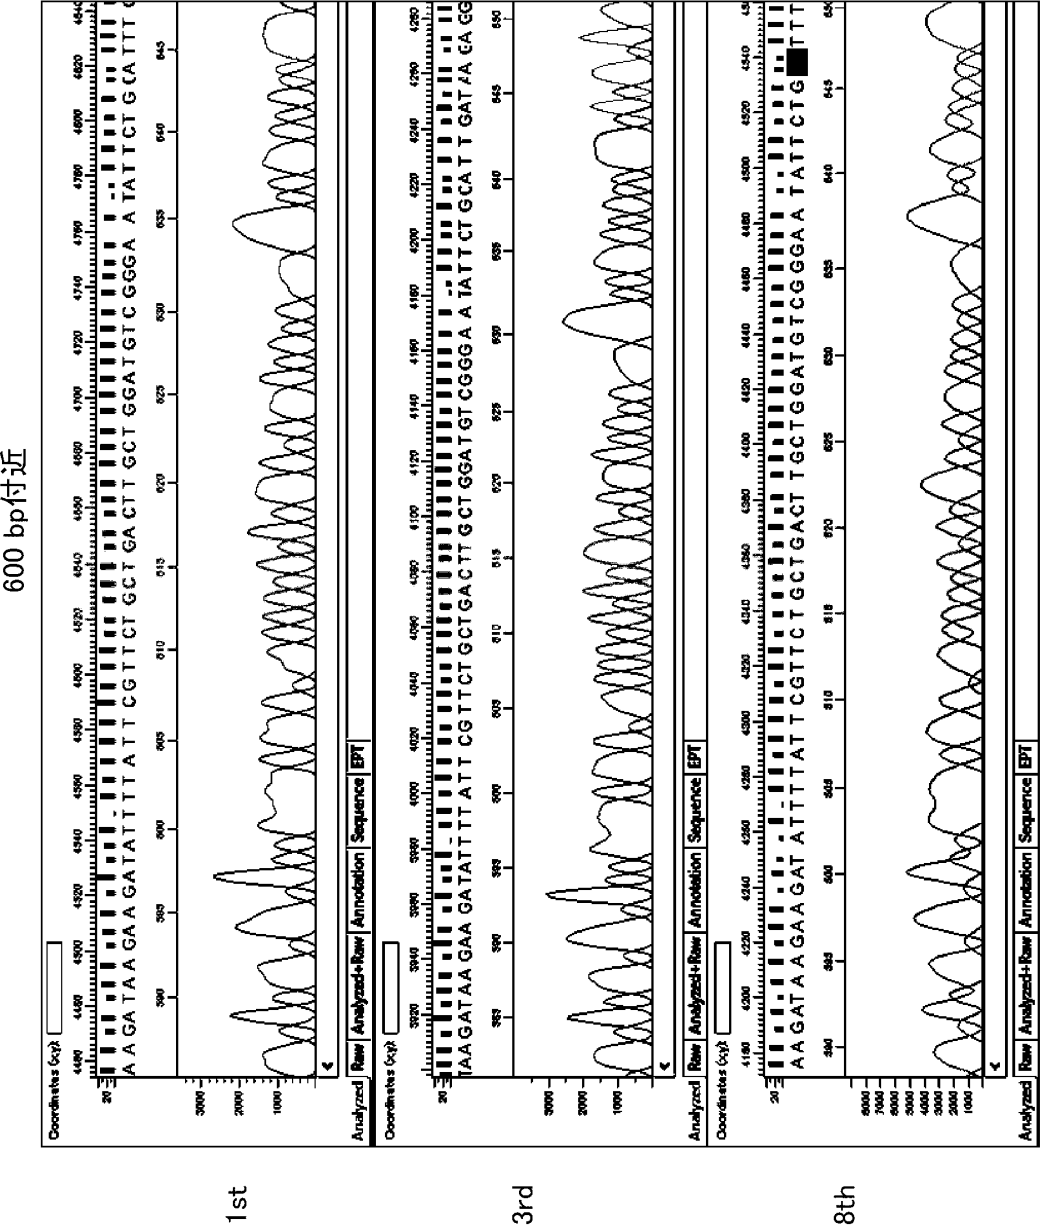


[図13]

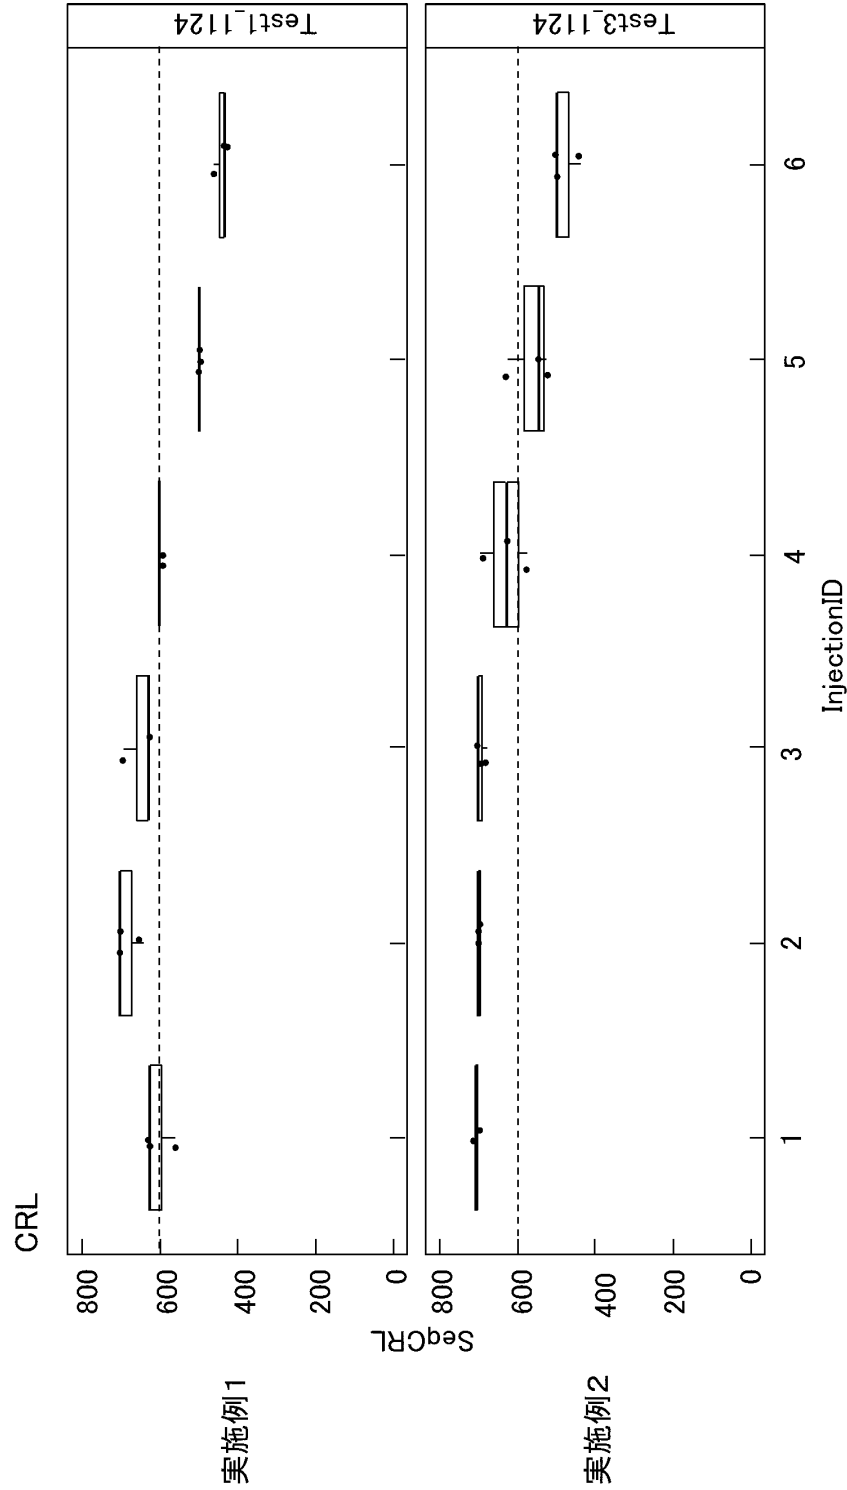


[図14]

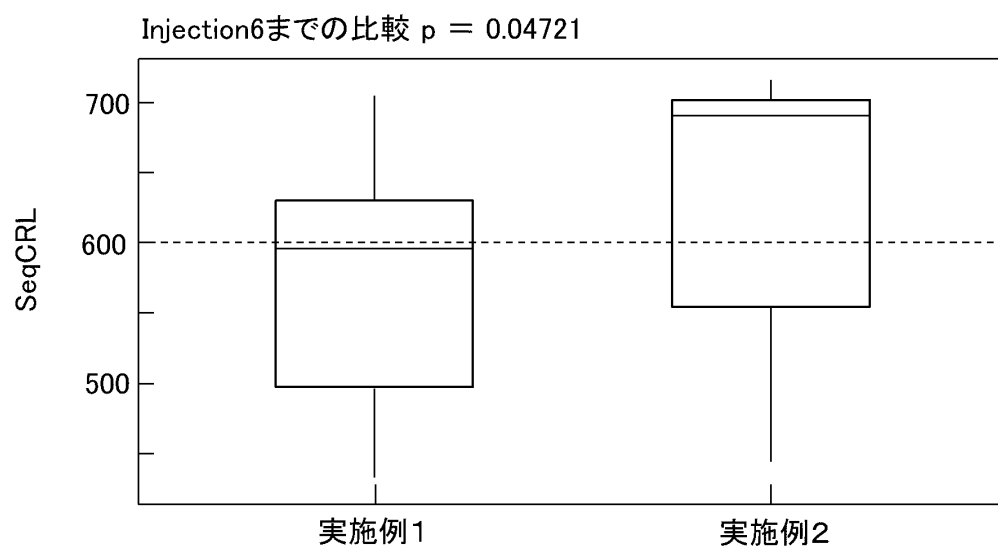

[図15]


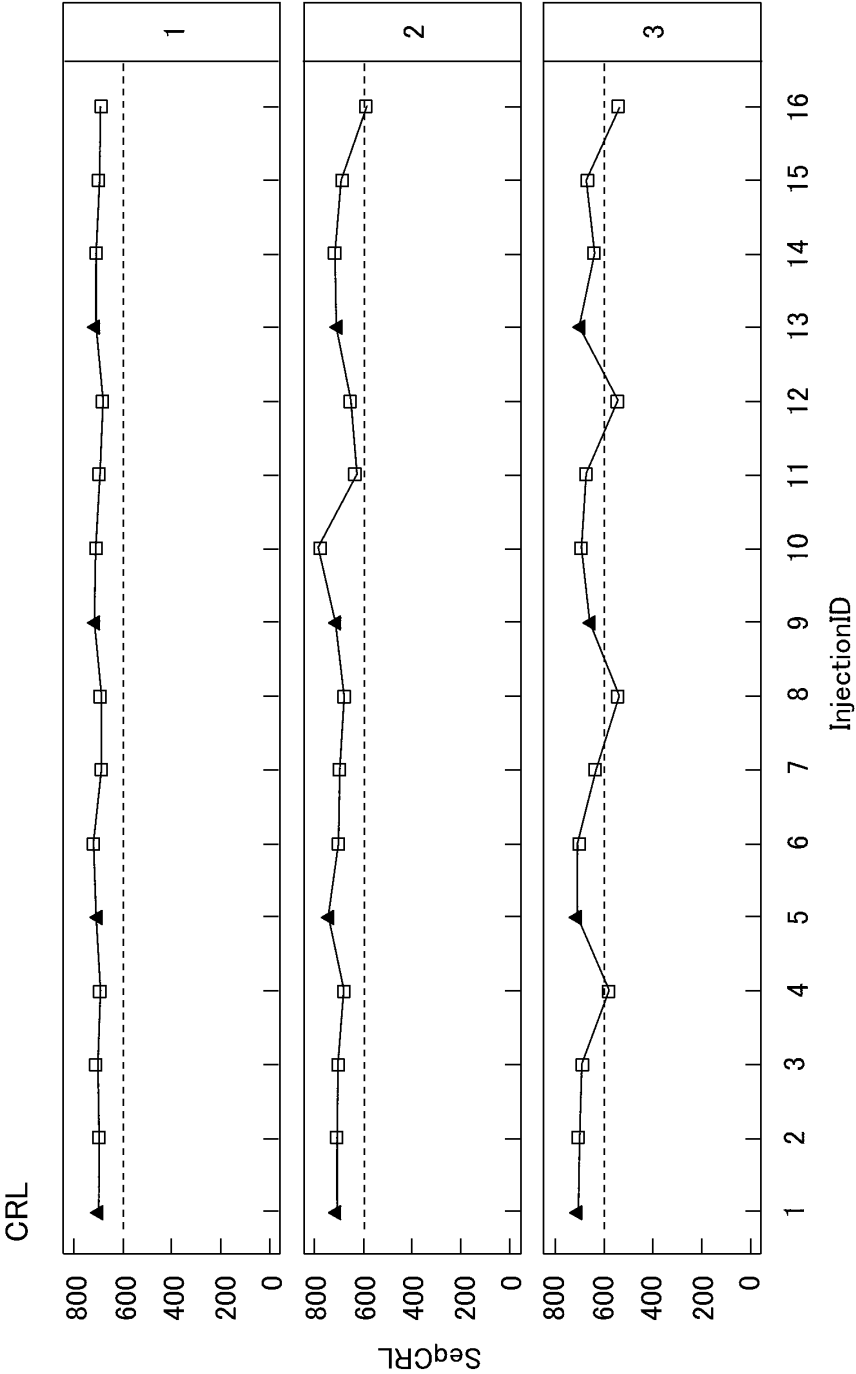


[図16]

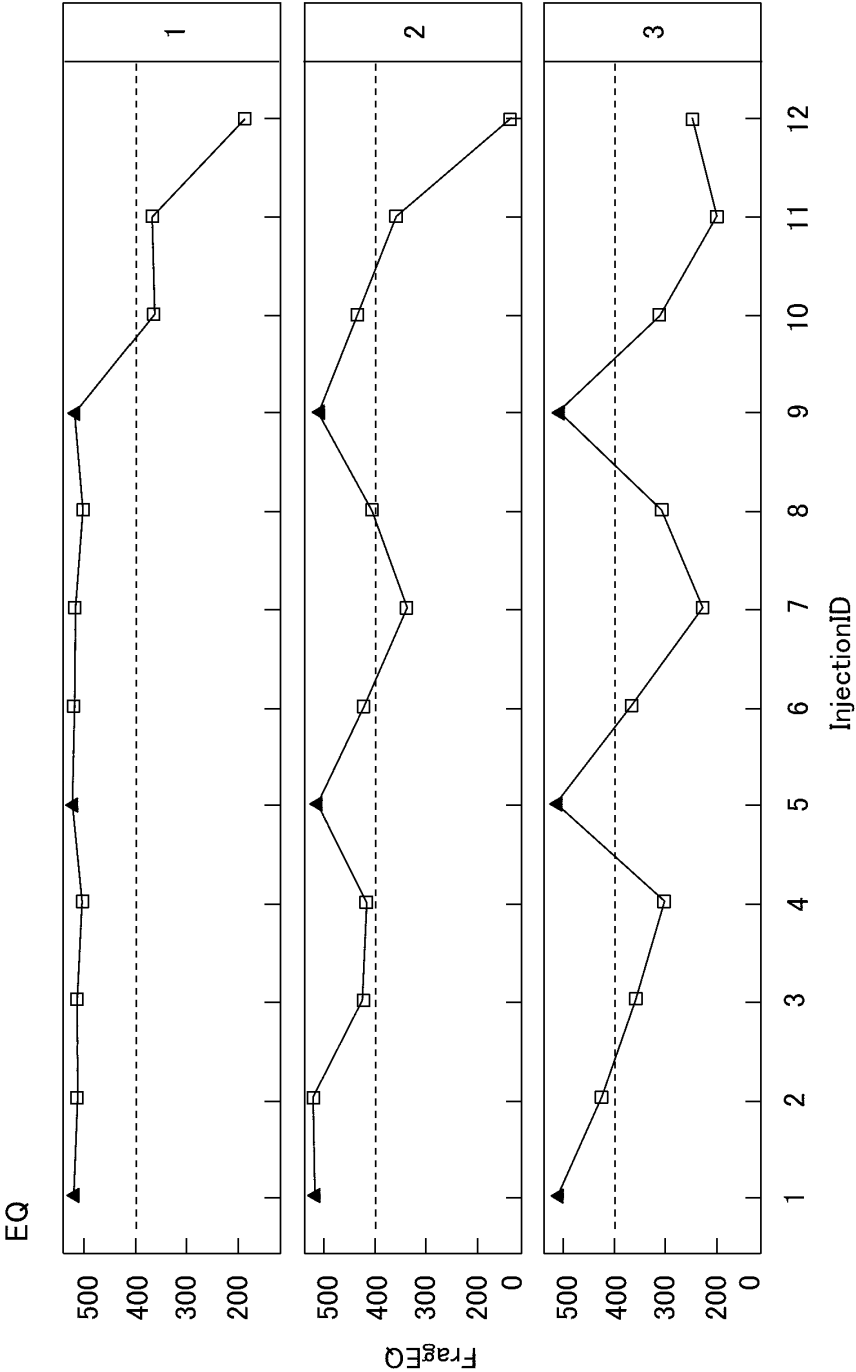

[図17]

実施例1, 実施例3 B

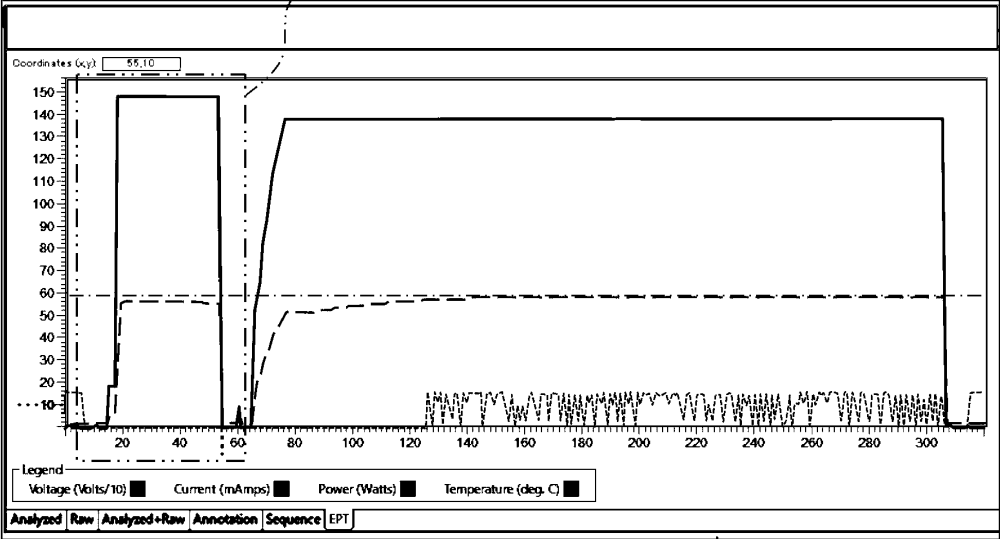

実施例2, 実施例4

