

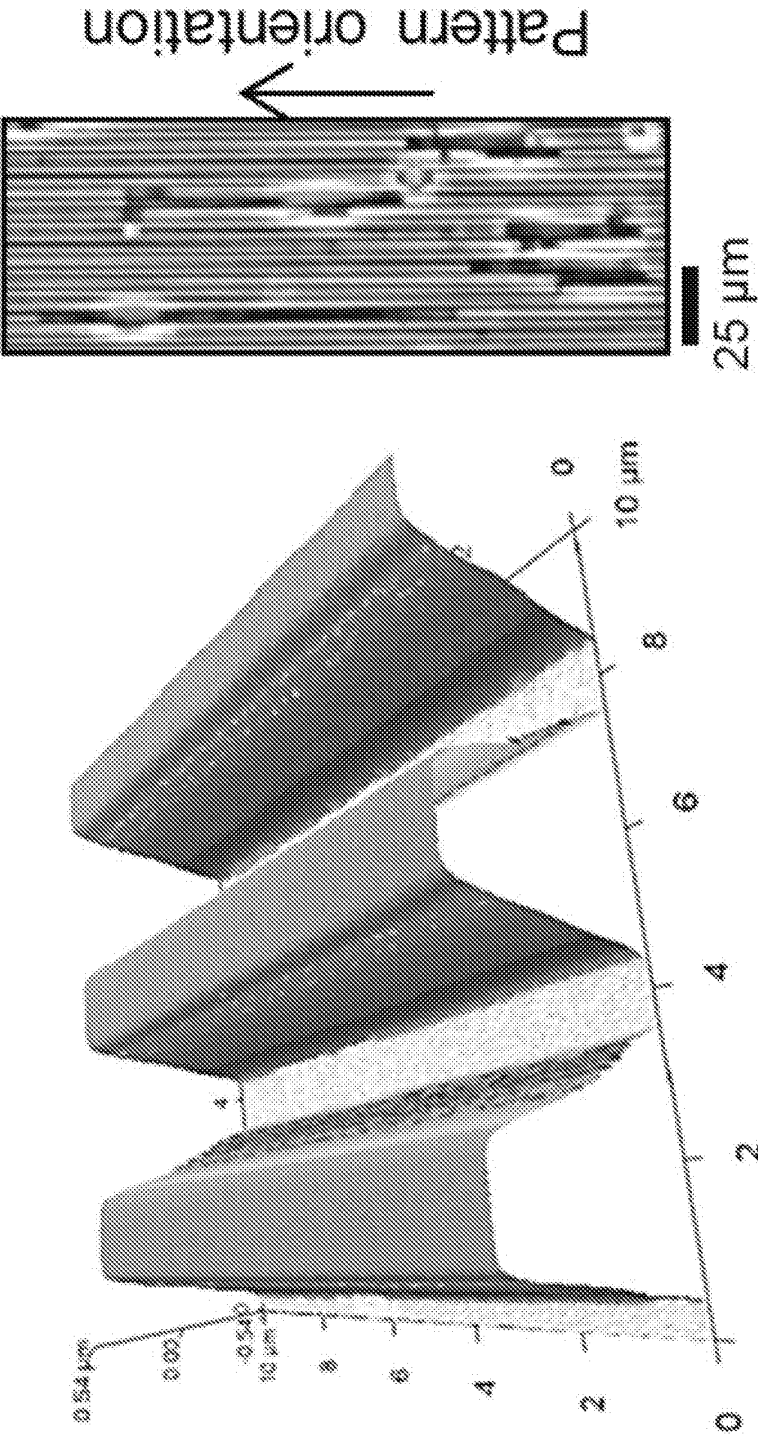


FIG. 1A

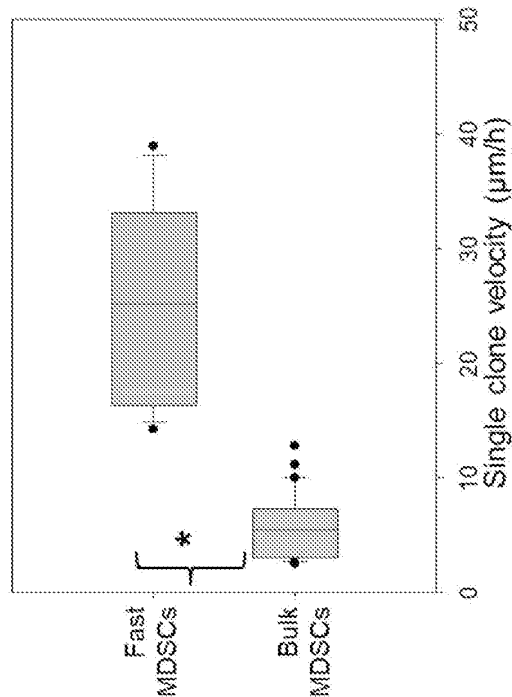


FIG. 1C

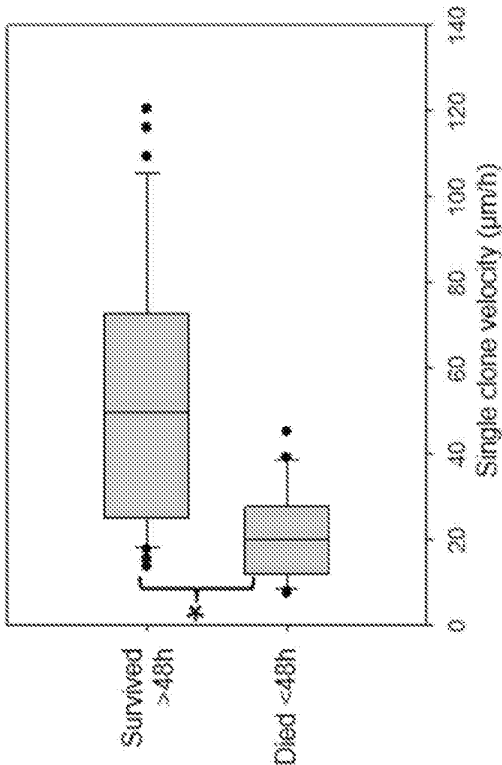


FIG. 1B

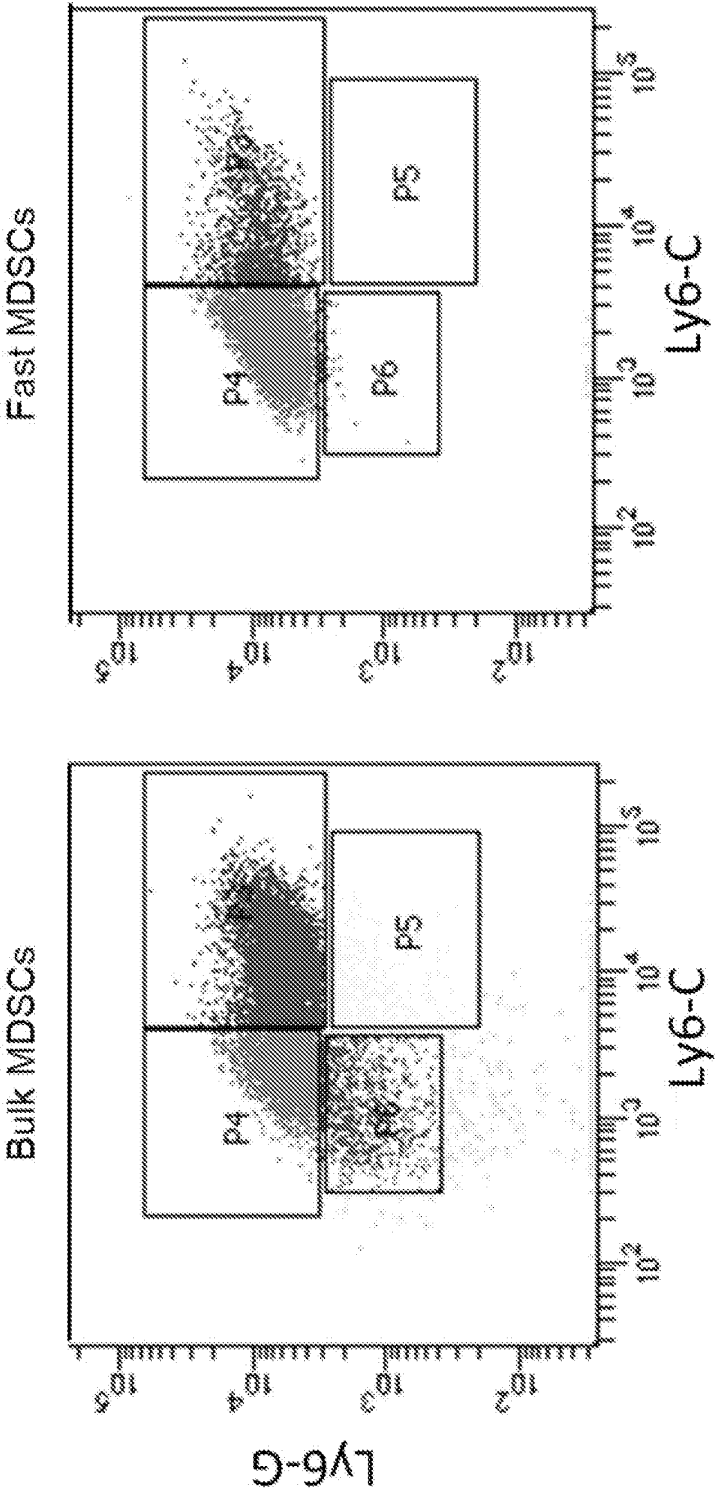


FIG. 1E

FIG. 1D

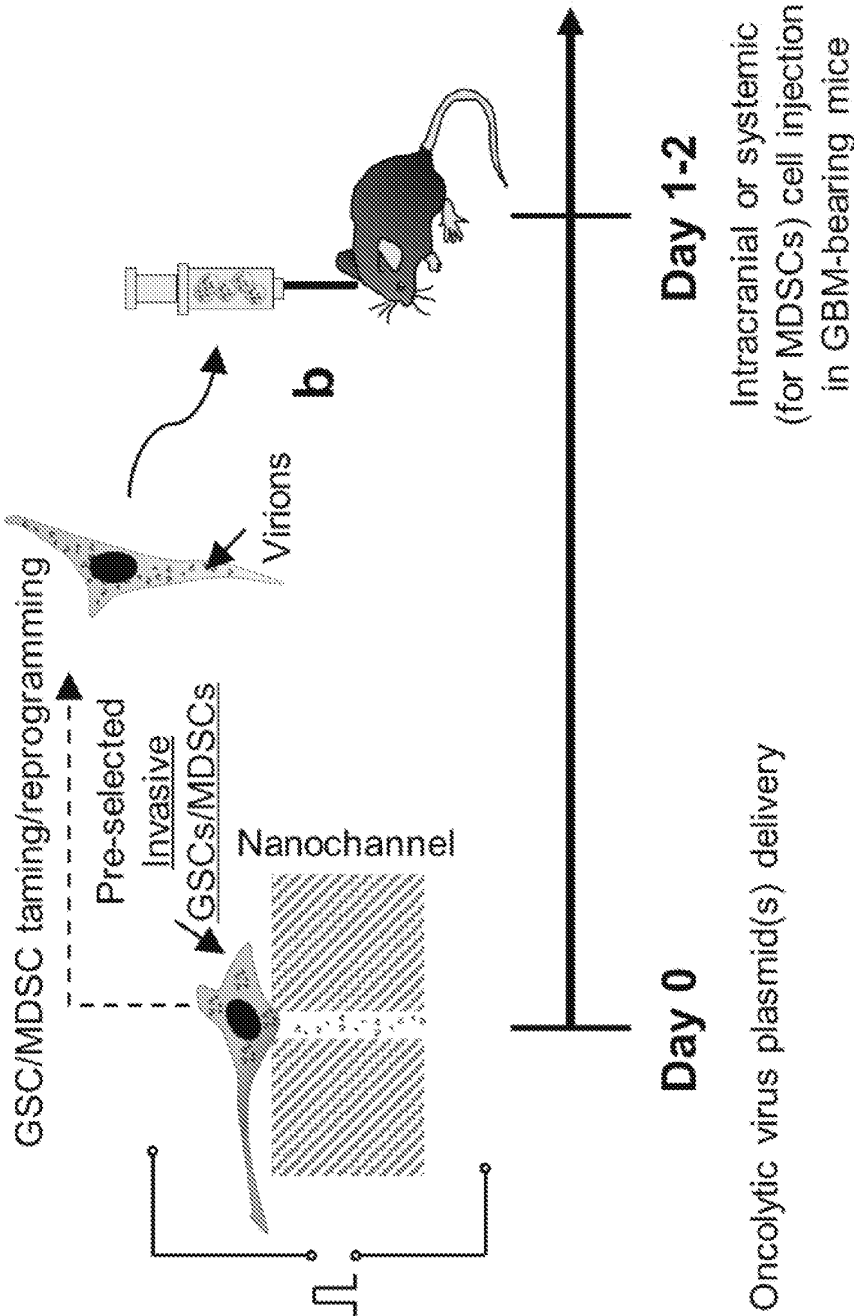


FIG. 2

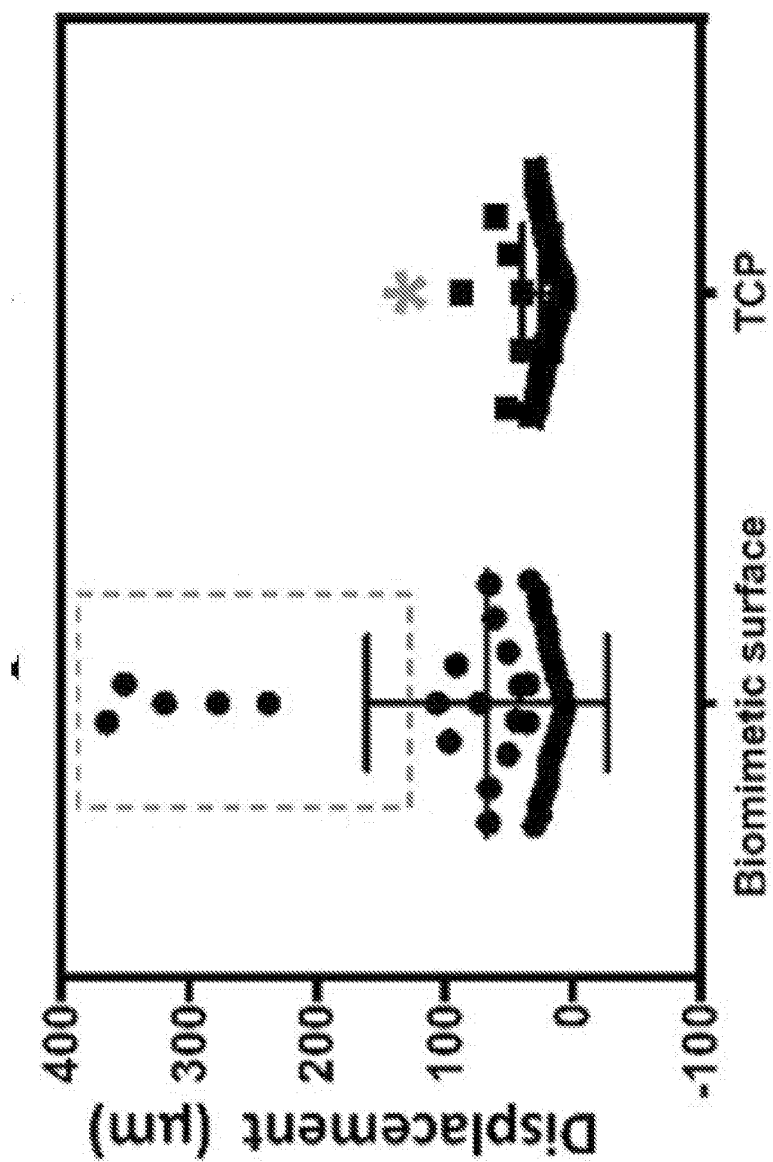


FIG. 3

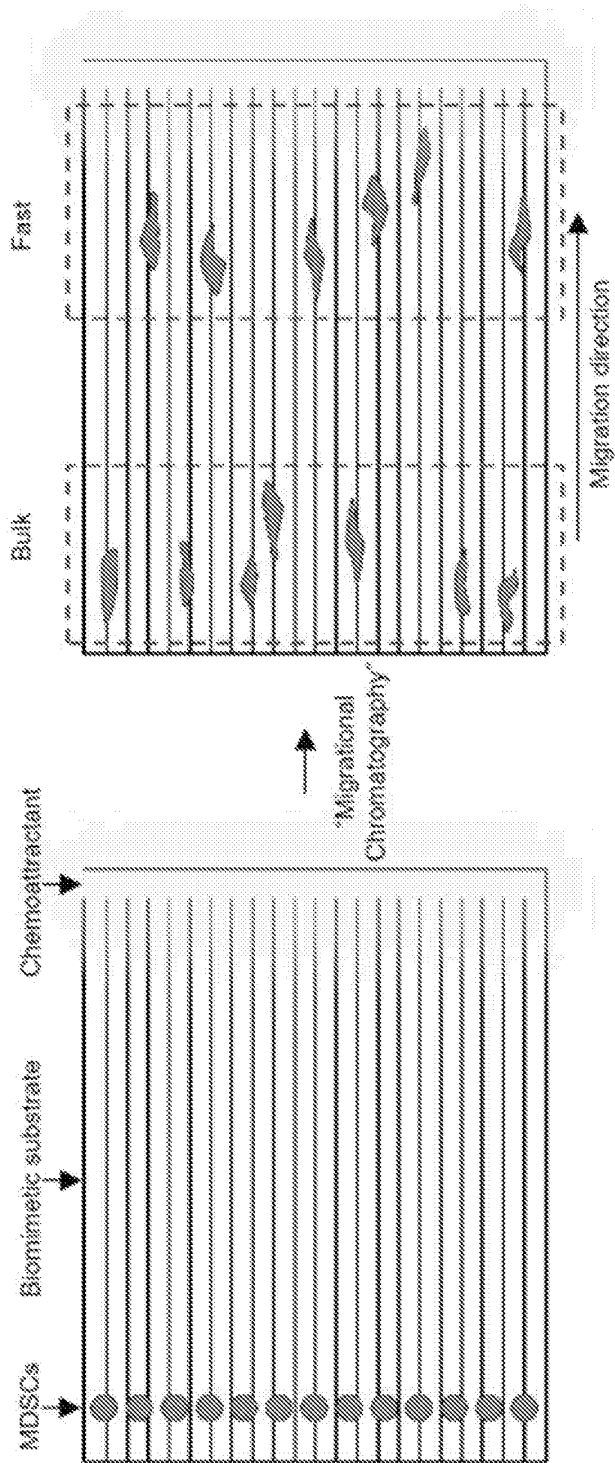


FIG. 4A

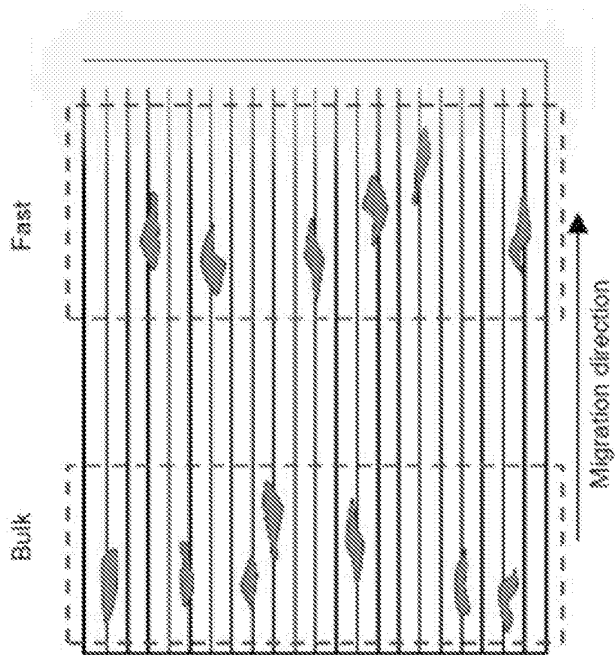


FIG. 4B

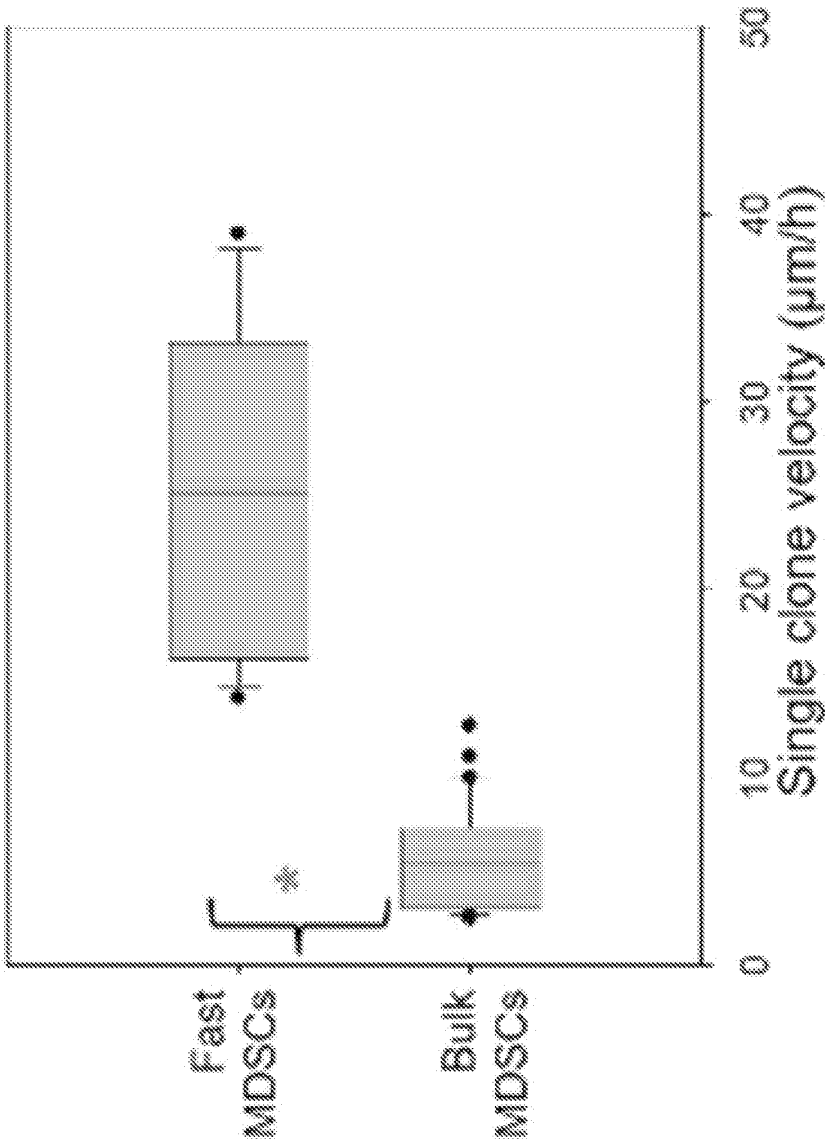


FIG. 4C

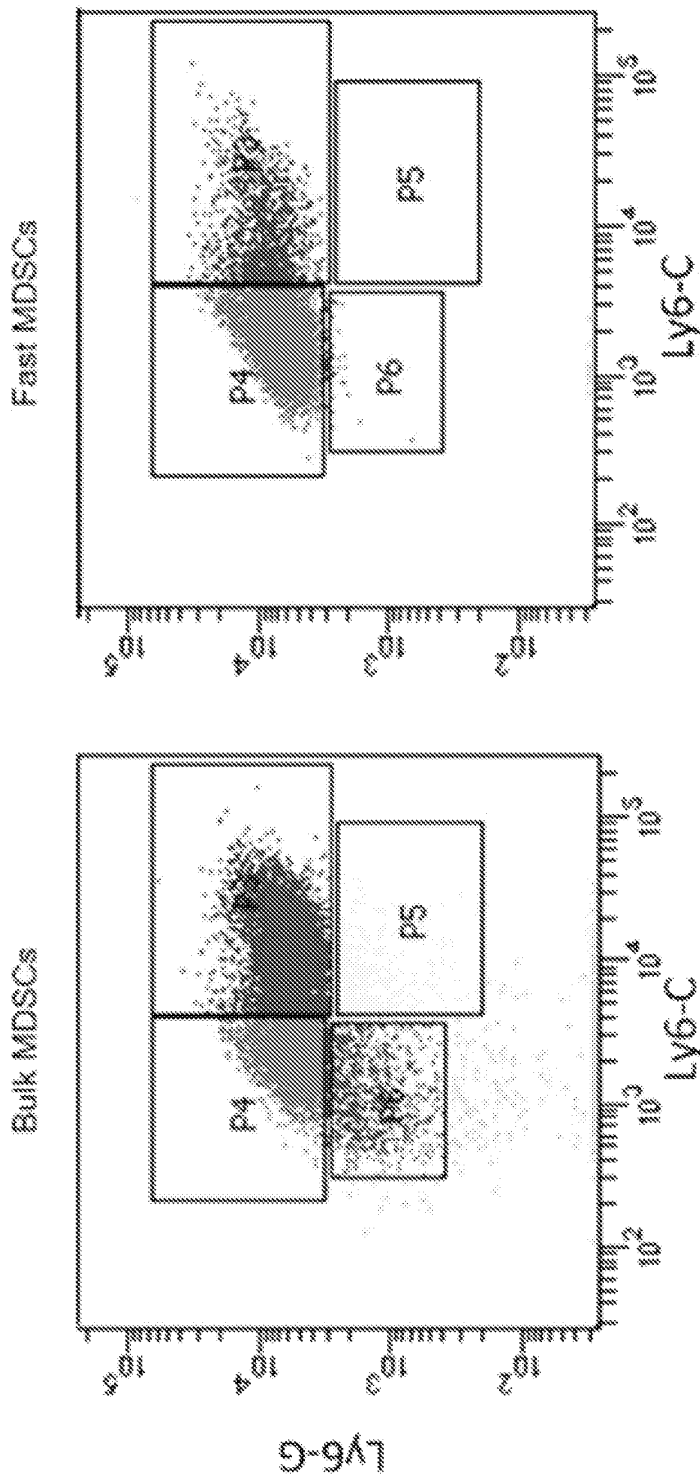


FIG. 4D

FIG. 4E

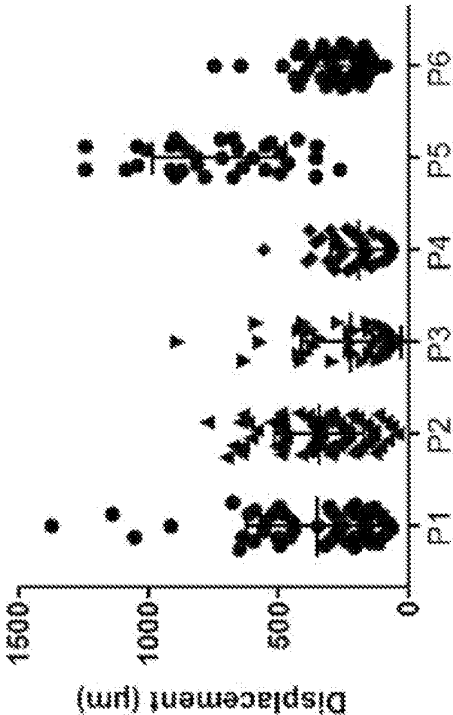


FIG. 5B

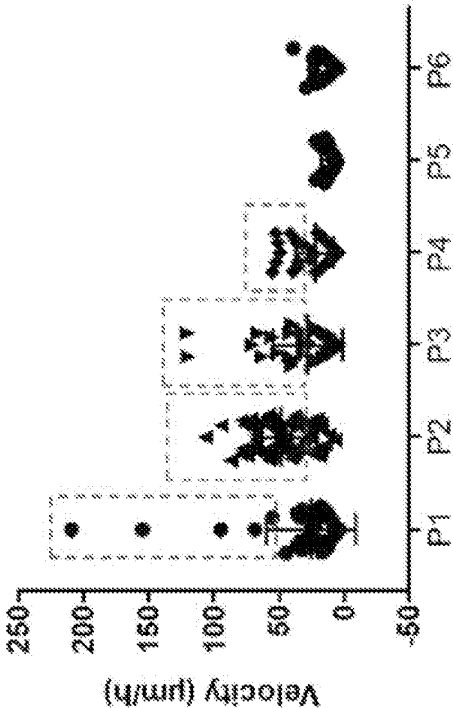


FIG. 5A

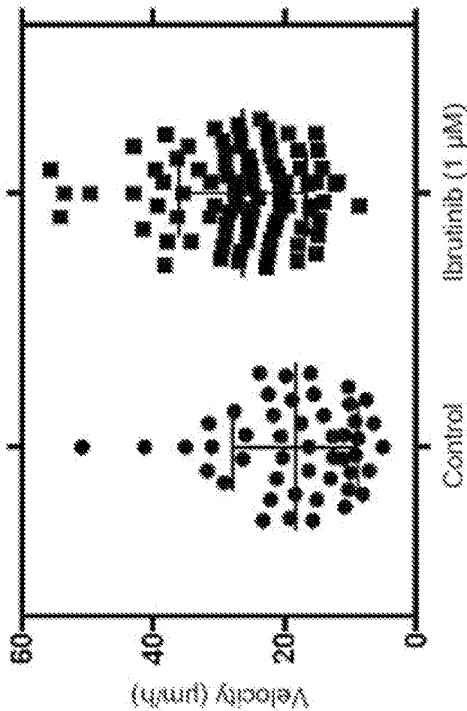


FIG. 6B

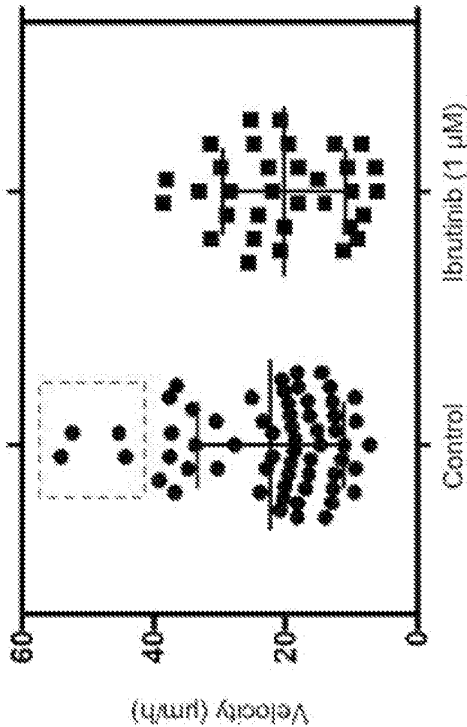


FIG. 6A


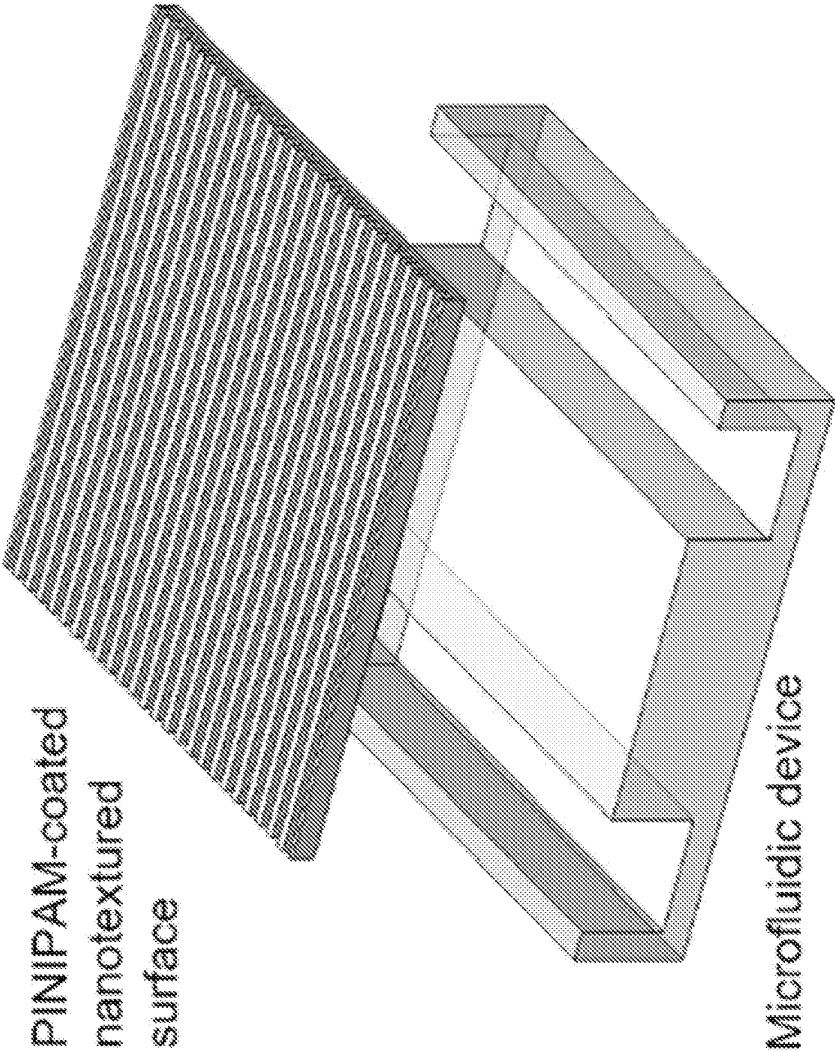


FIG. 7A

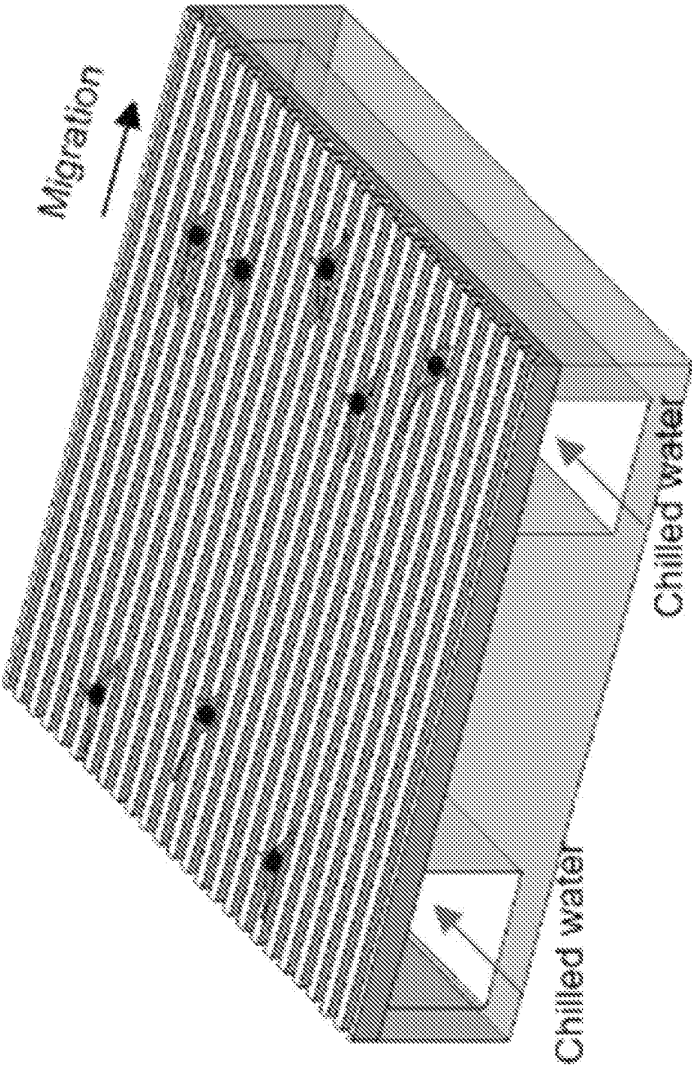

Assembled device for automated migrational chromatography

FIG. 7B

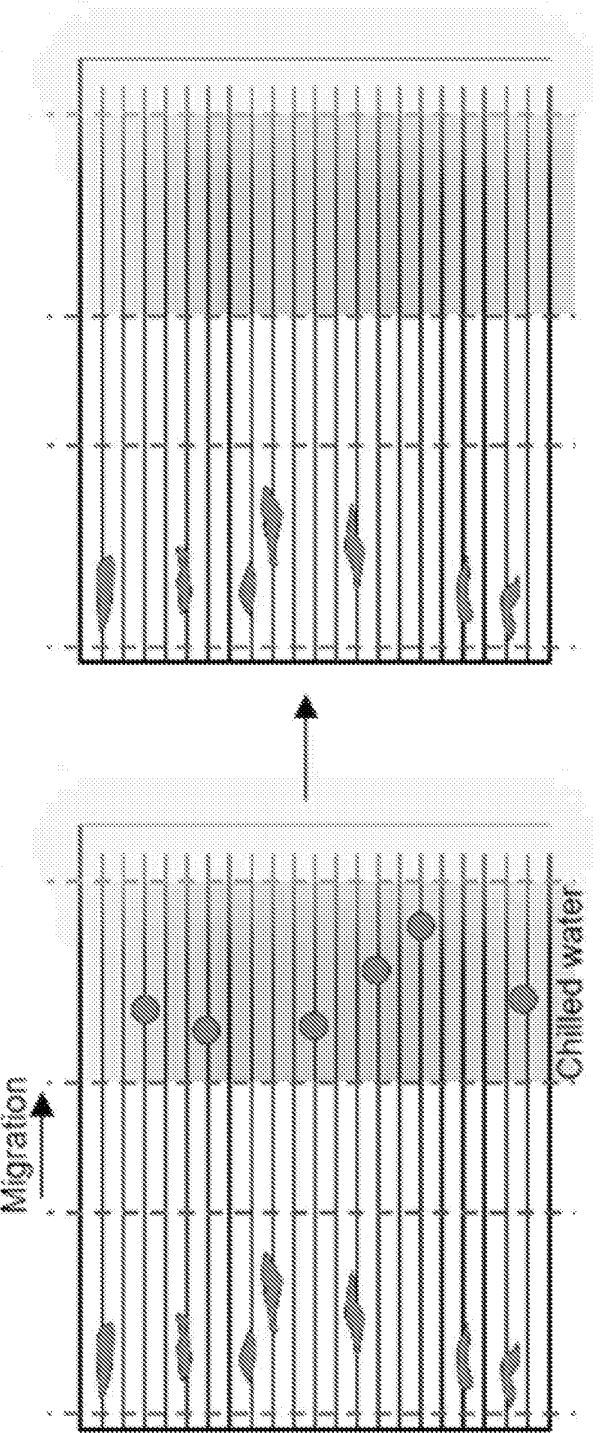


FIG. 7C

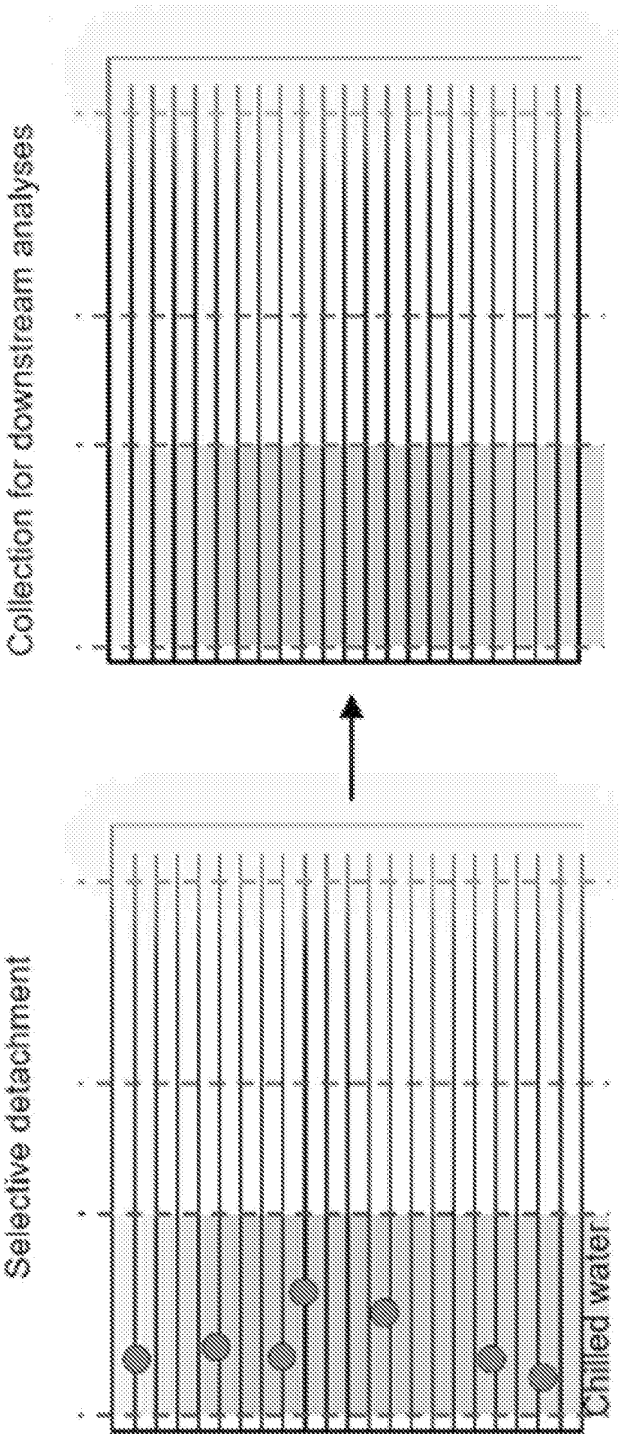


FIG. 7D

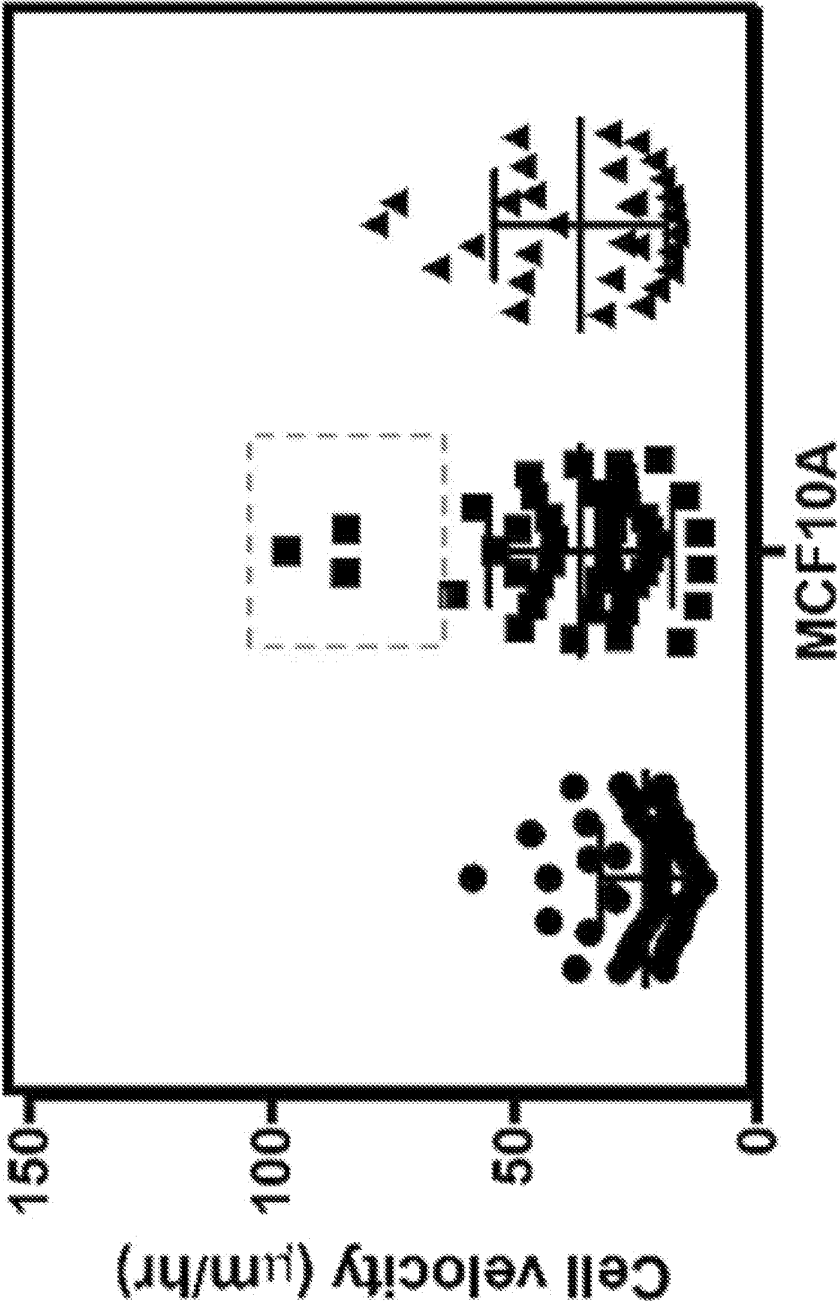


FIG. 8A

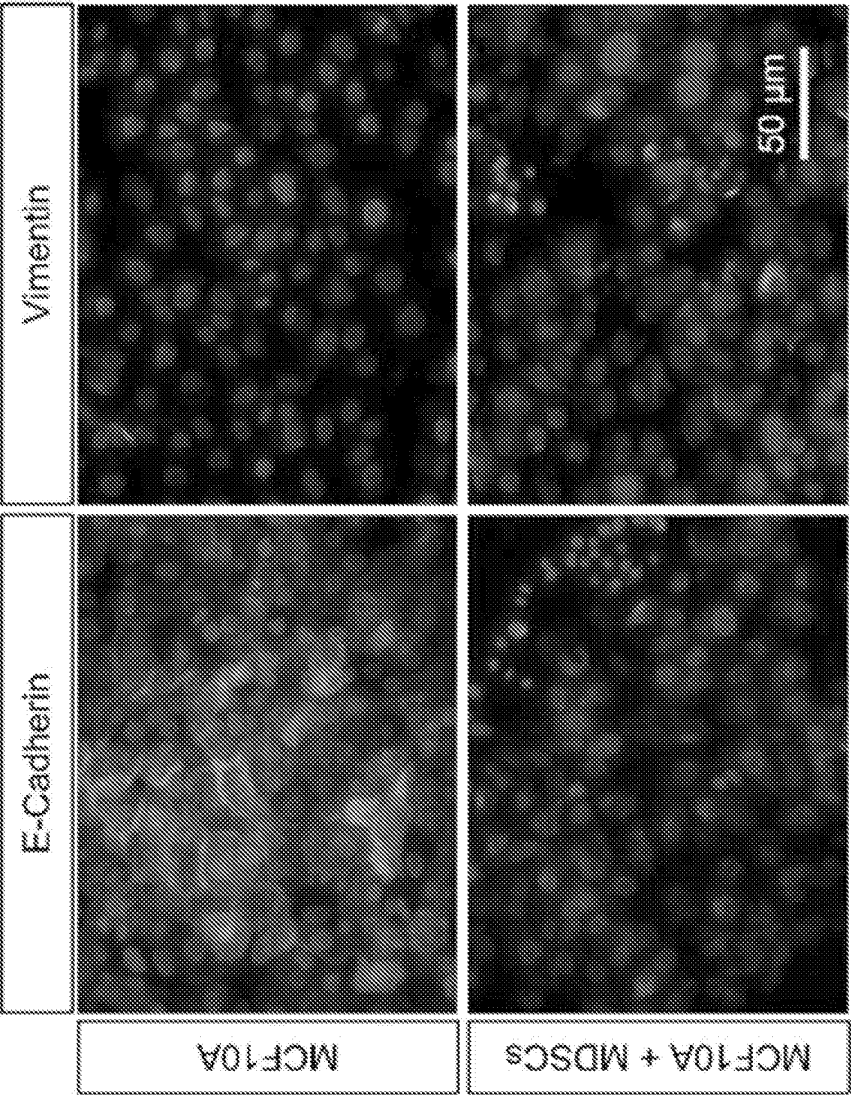


FIG. 8B

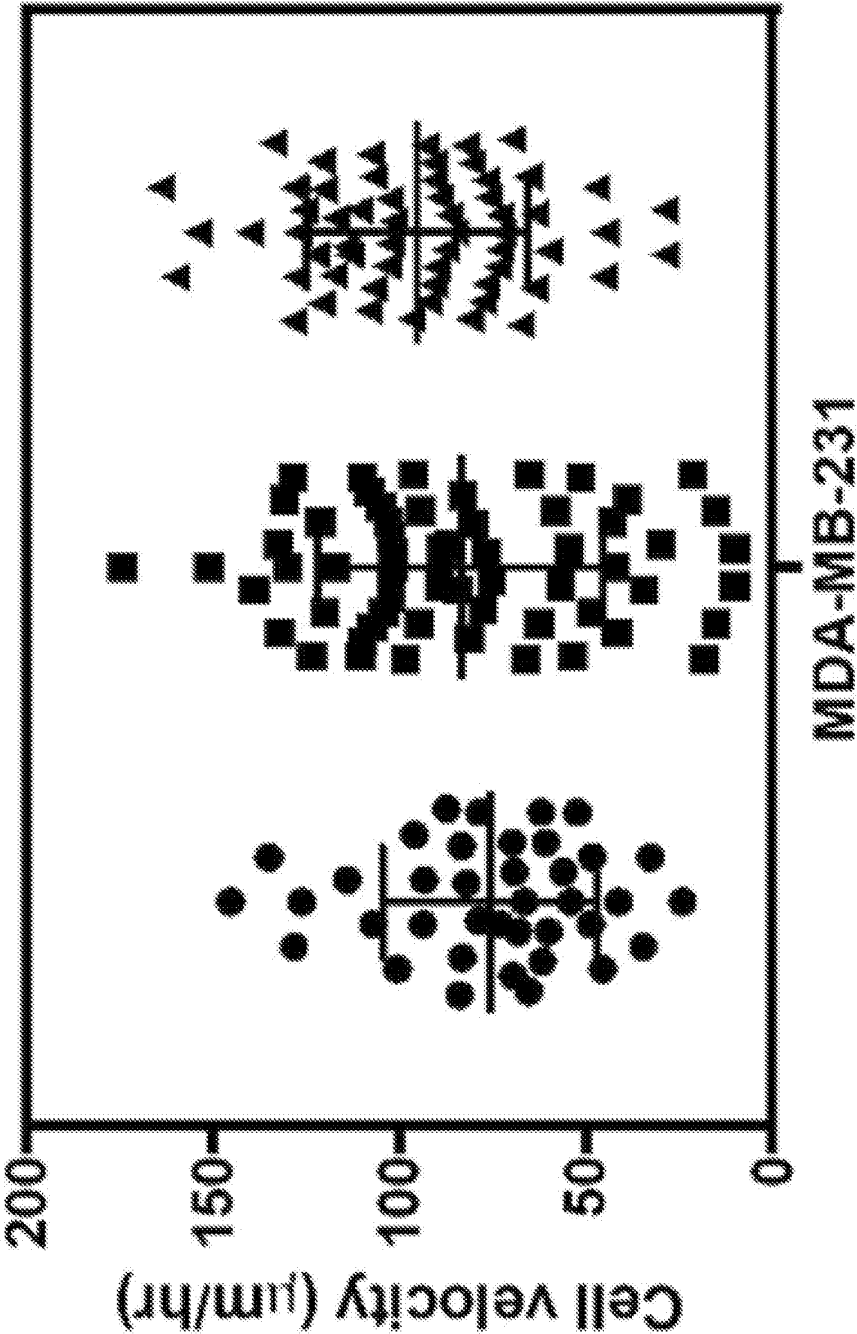


FIG. 8C

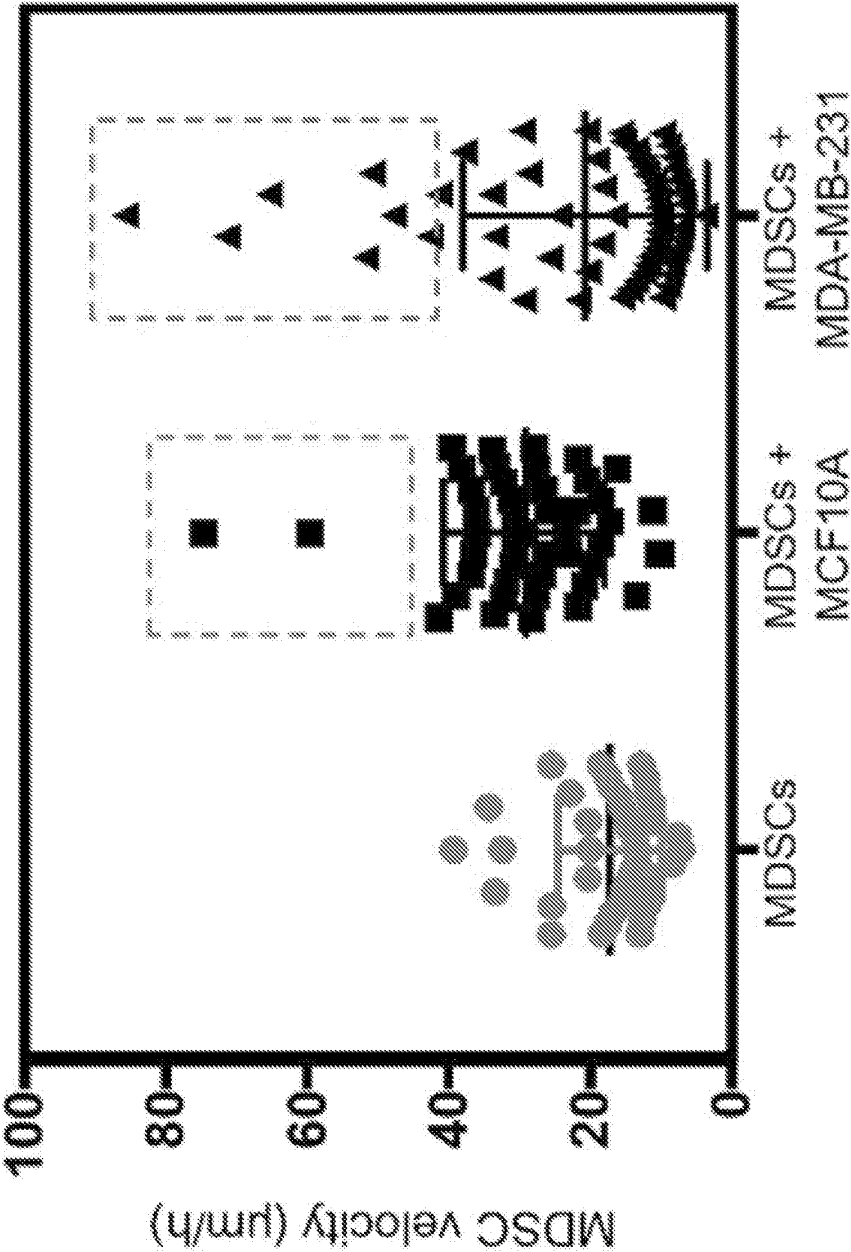


FIG. 9

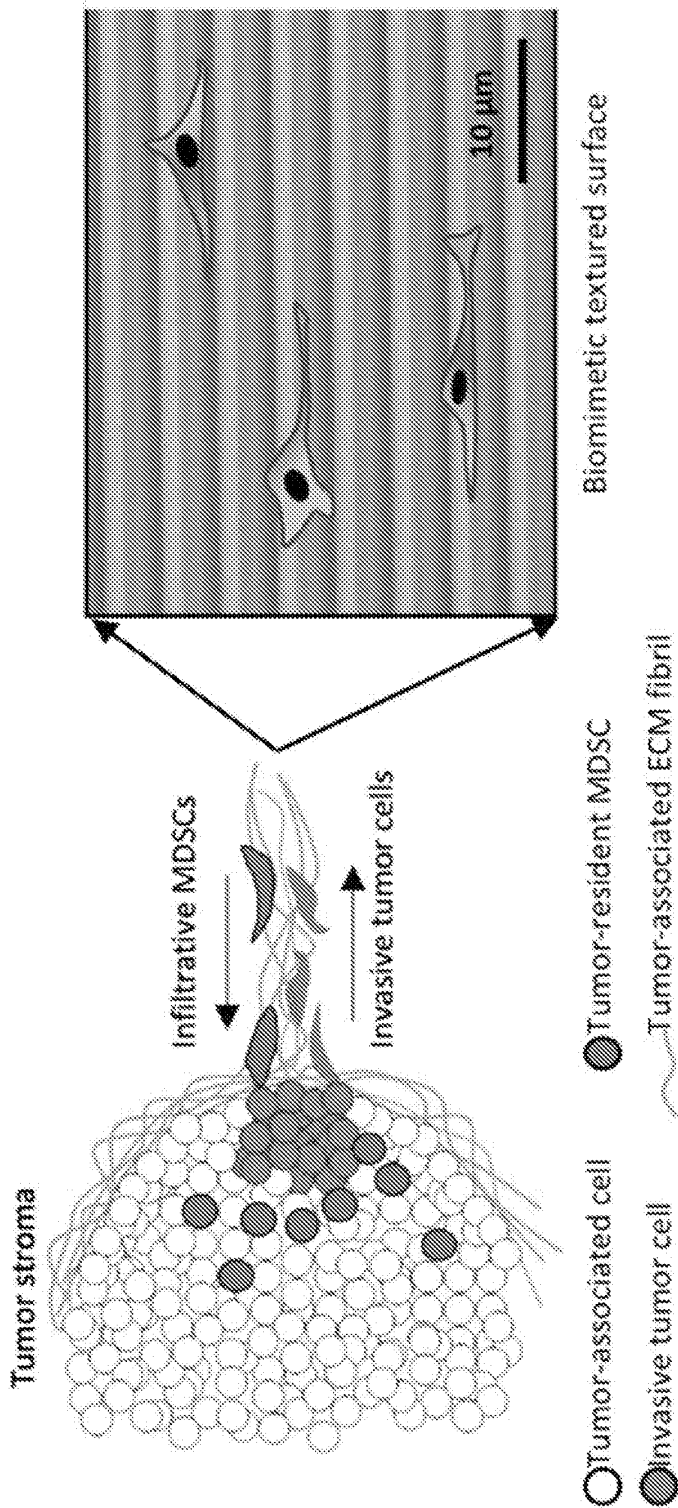


FIG. 10A

FIG. 10B

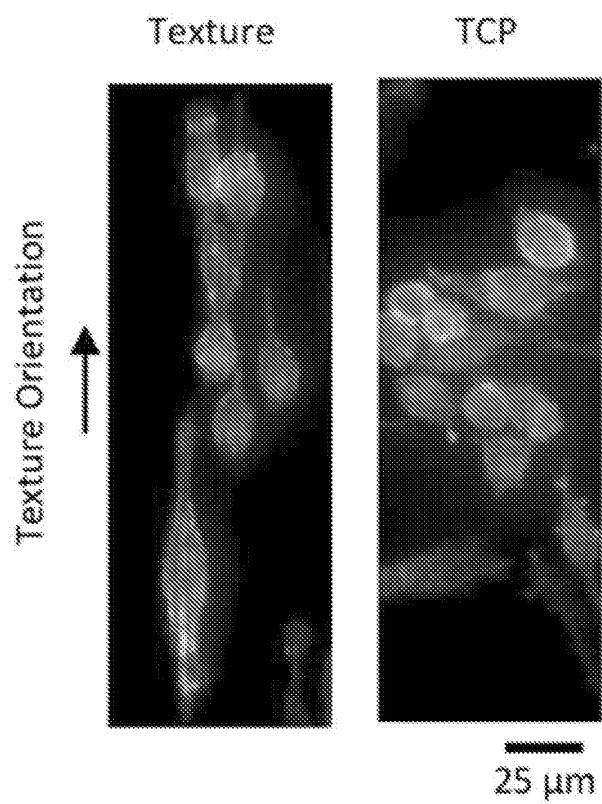


FIG. 10C

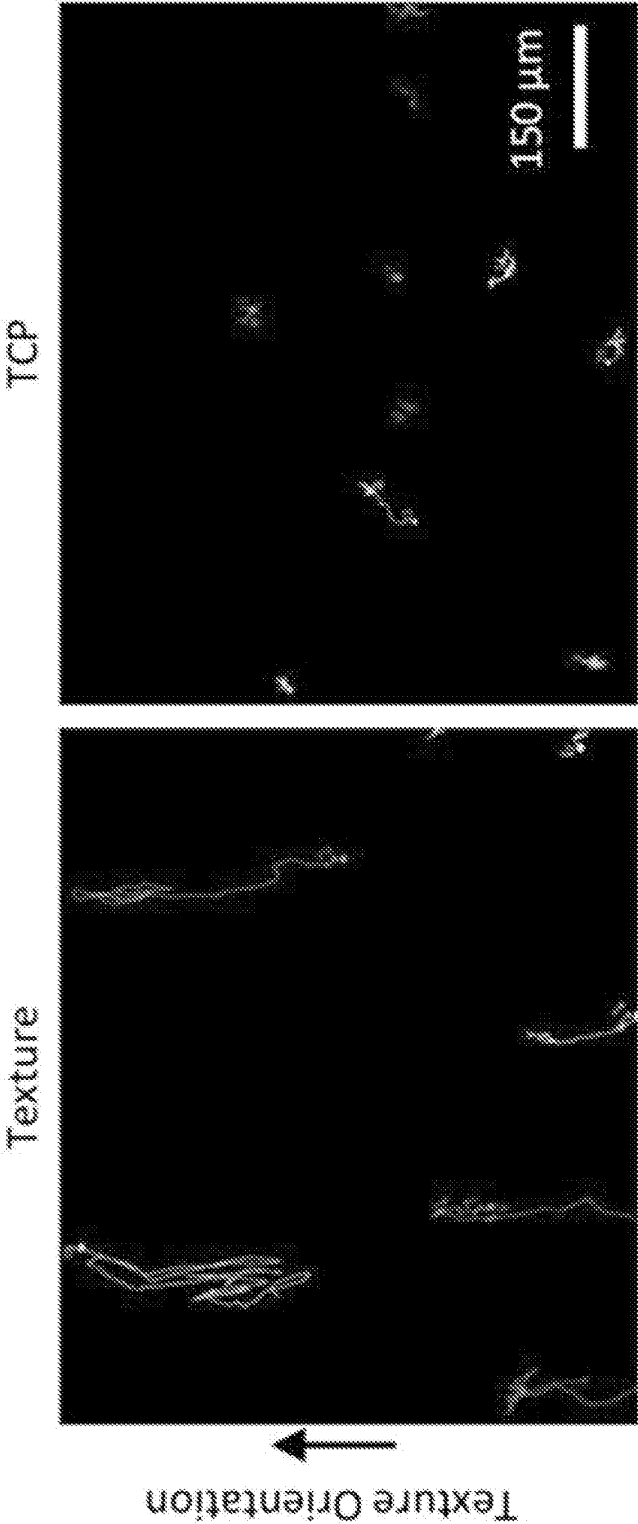


FIG. 10D

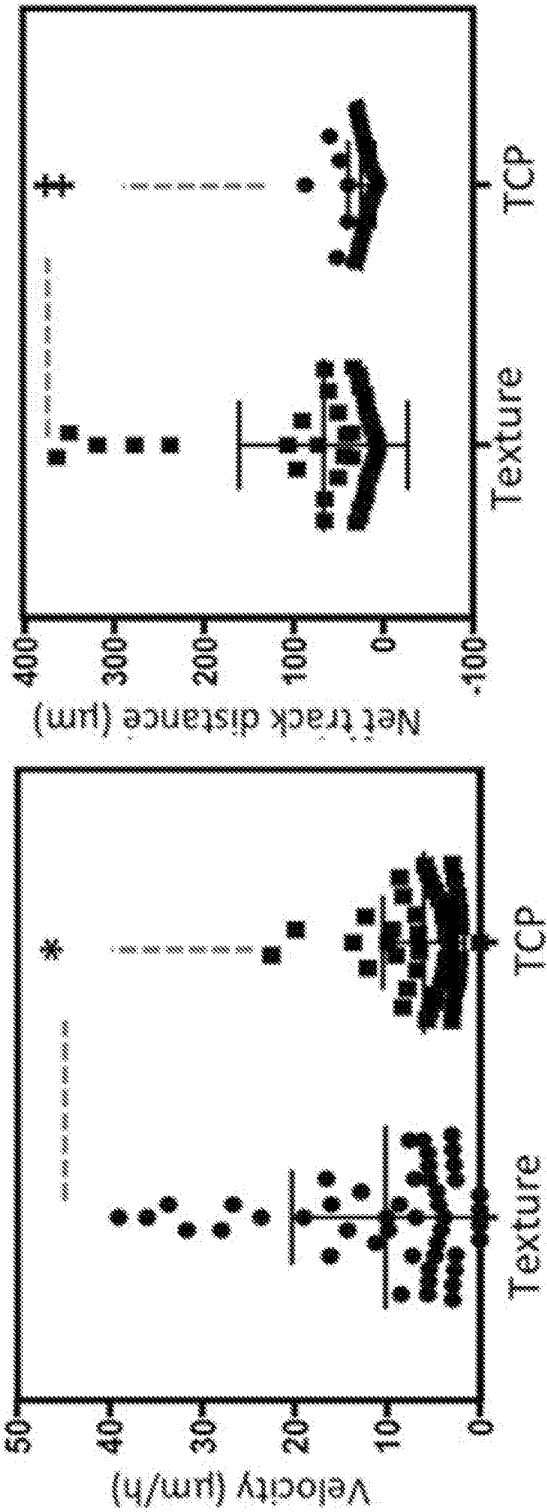


FIG. 10E

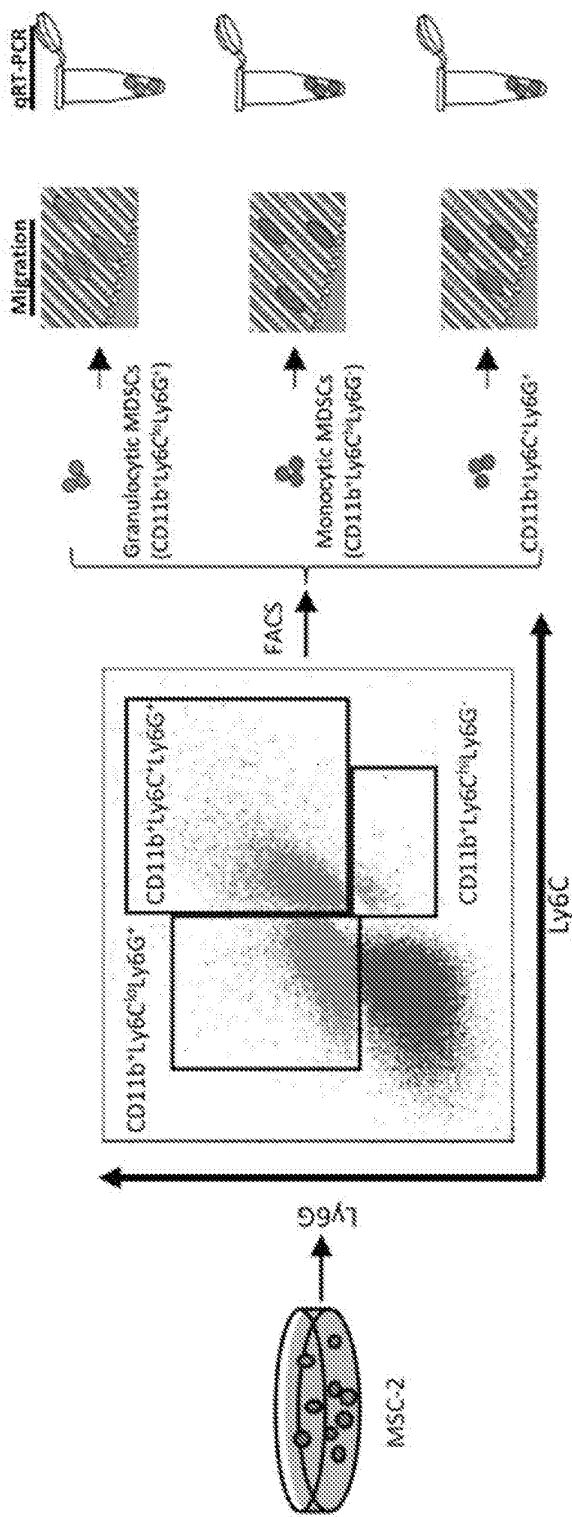


FIG. 11A

FIG. 11B

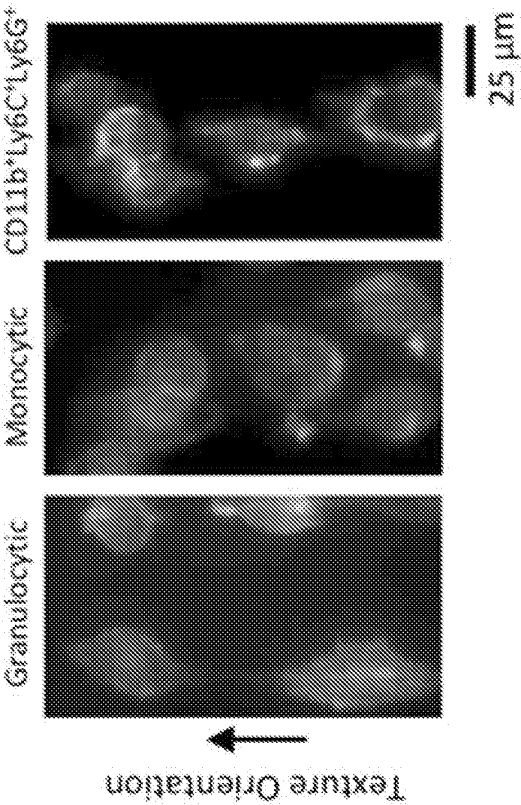


FIG. 11C

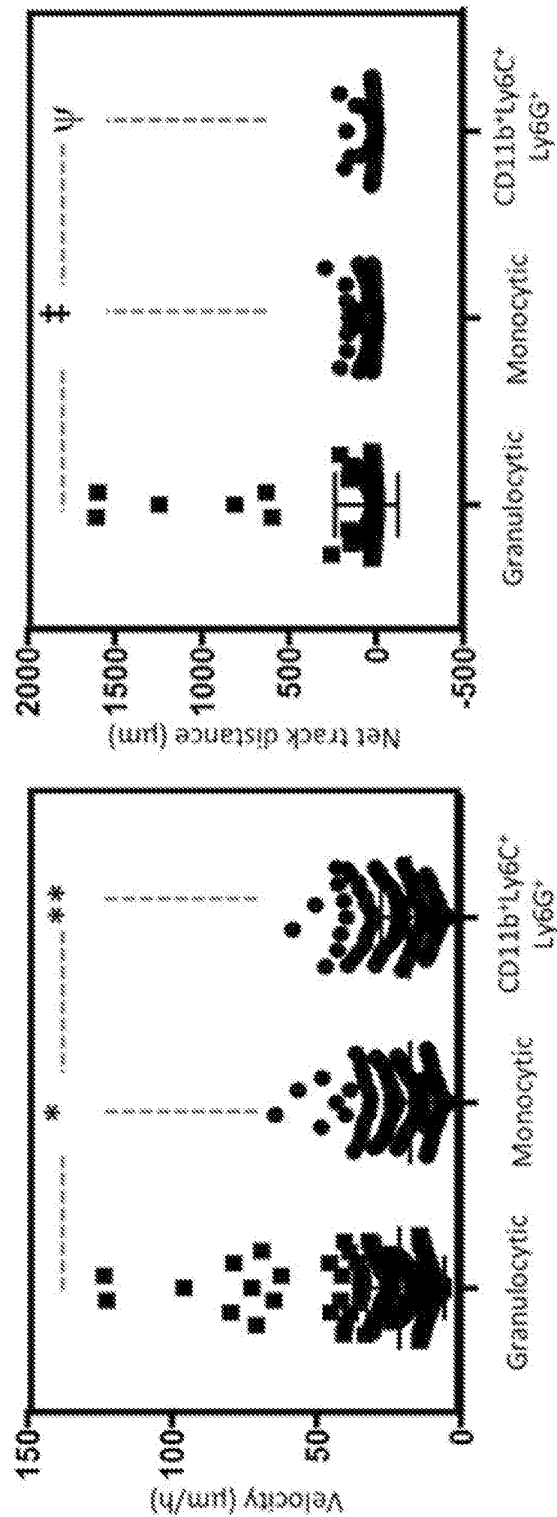


FIG. 11D

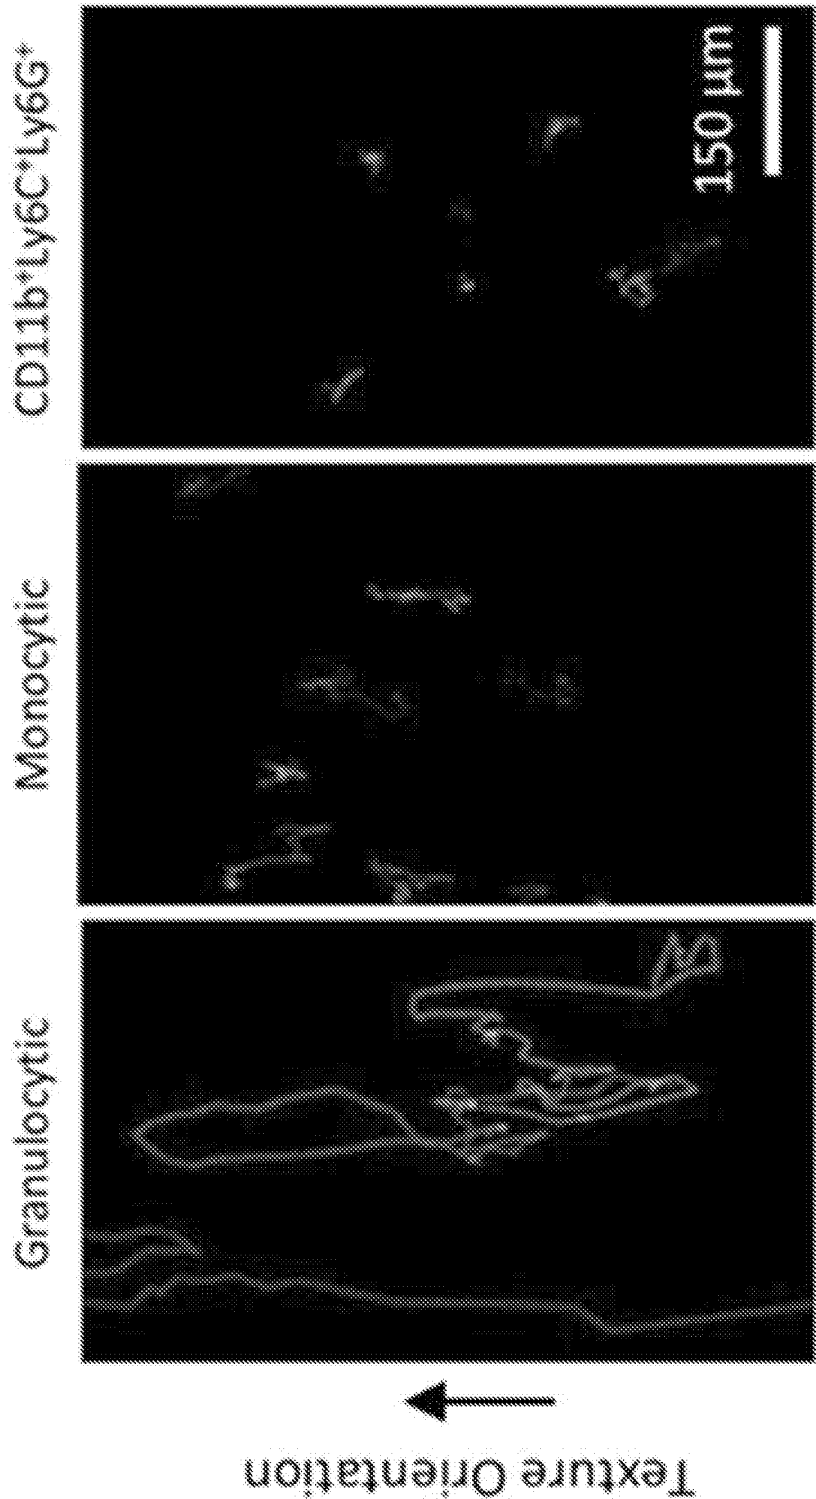


FIG. 11E

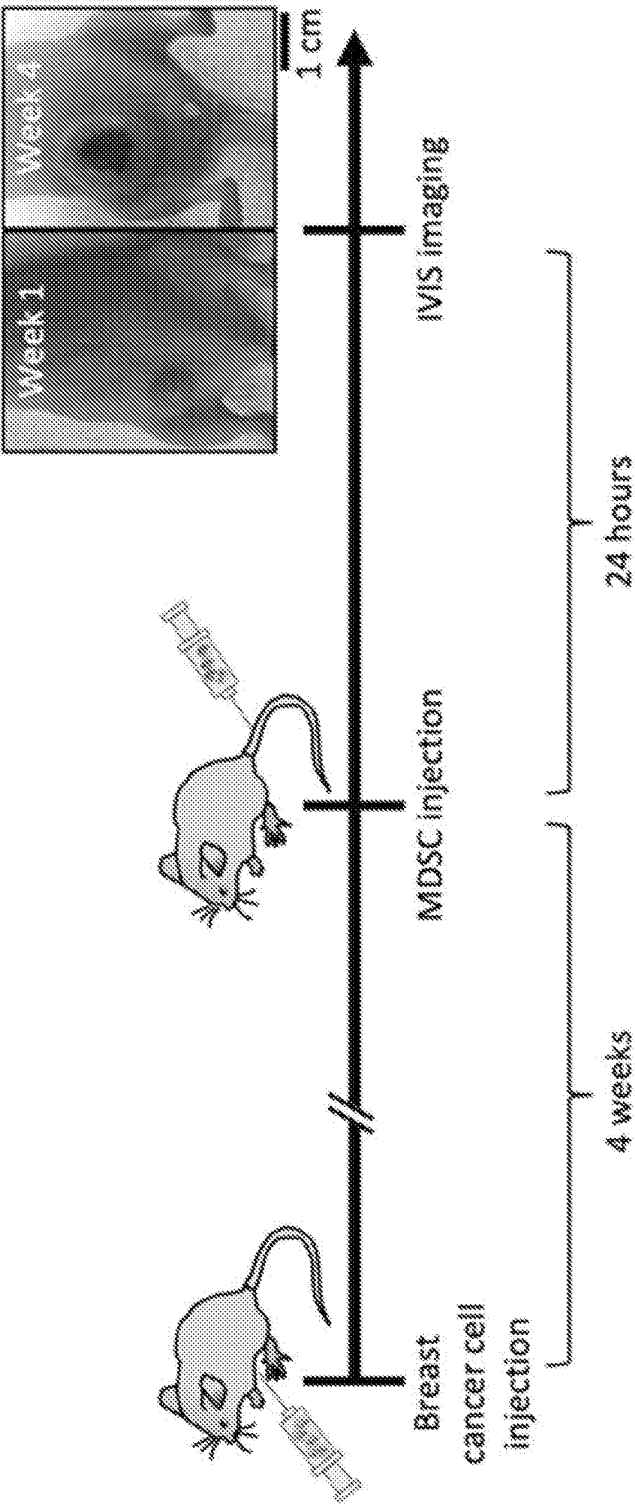


FIG. 11F

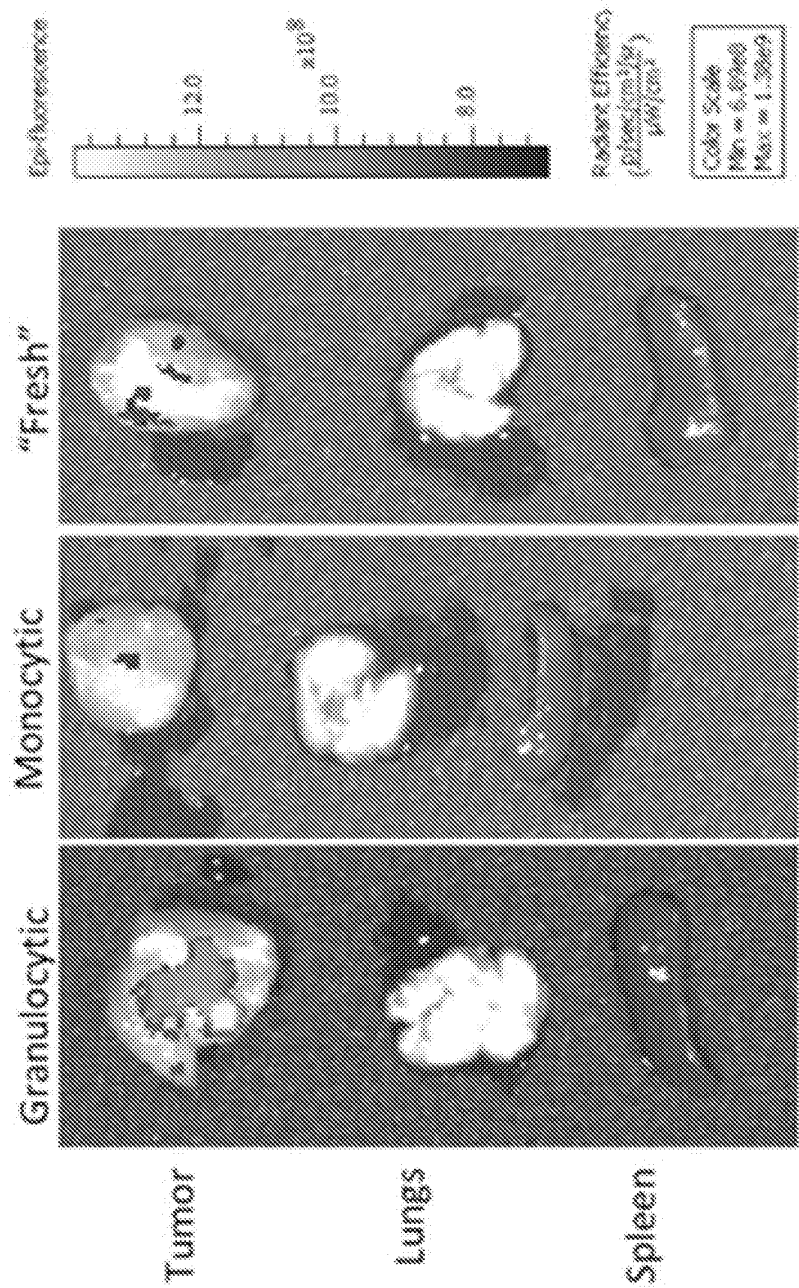


FIG. 11G

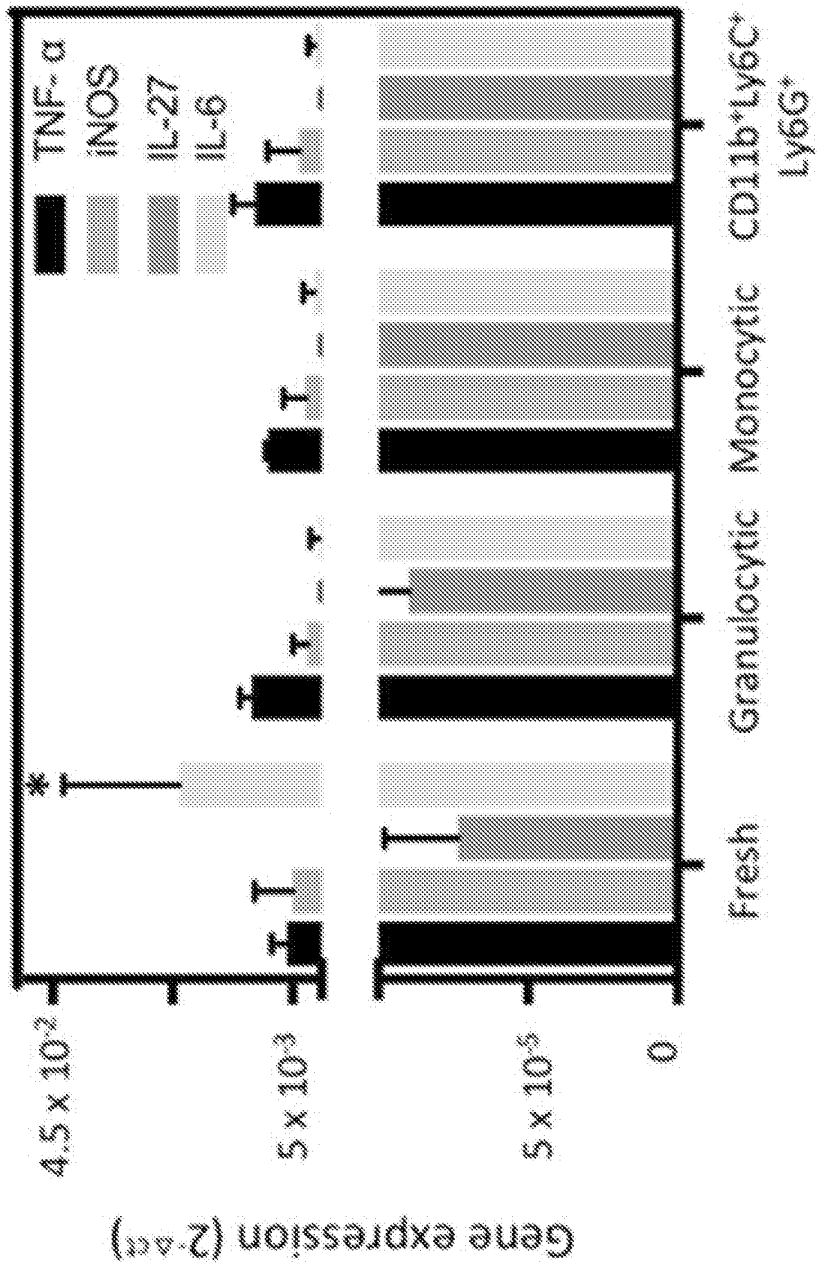


FIG. 11H

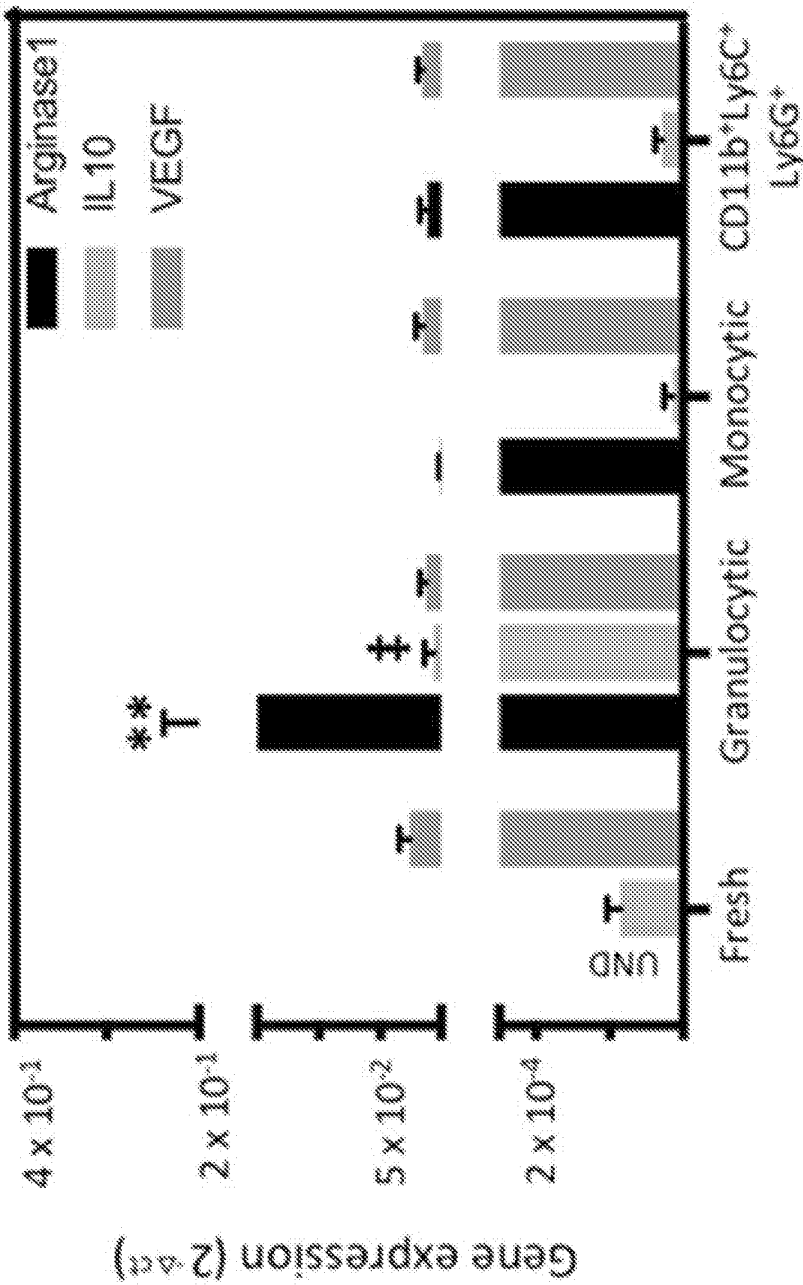


FIG. 11I

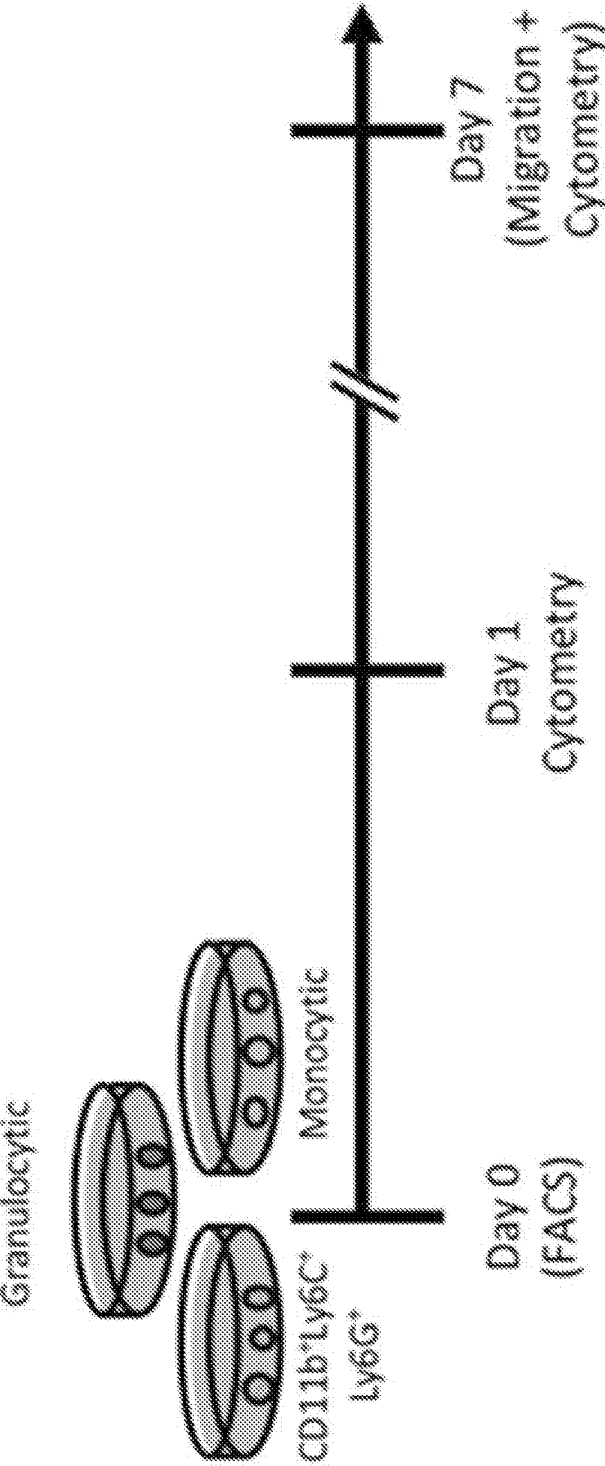


FIG. 12A

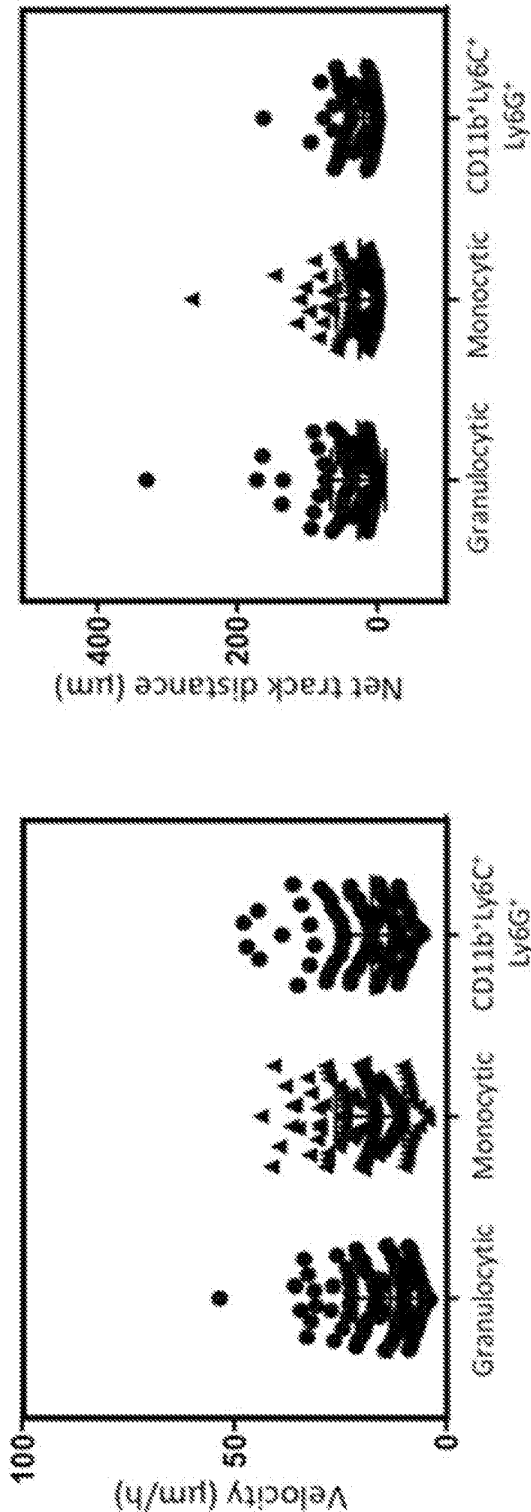


FIG. 12B

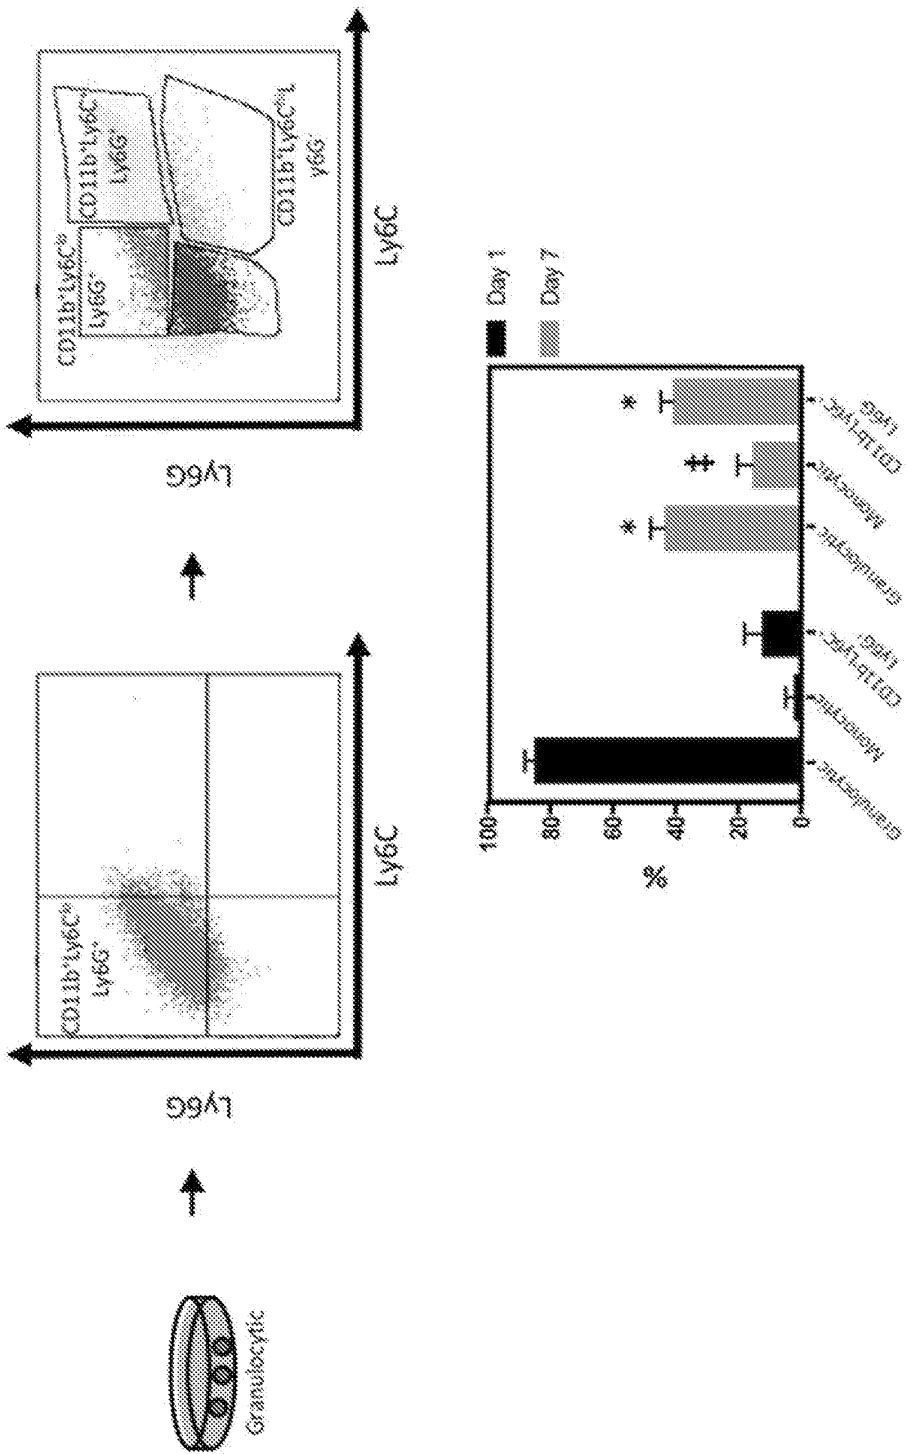


FIG. 12C

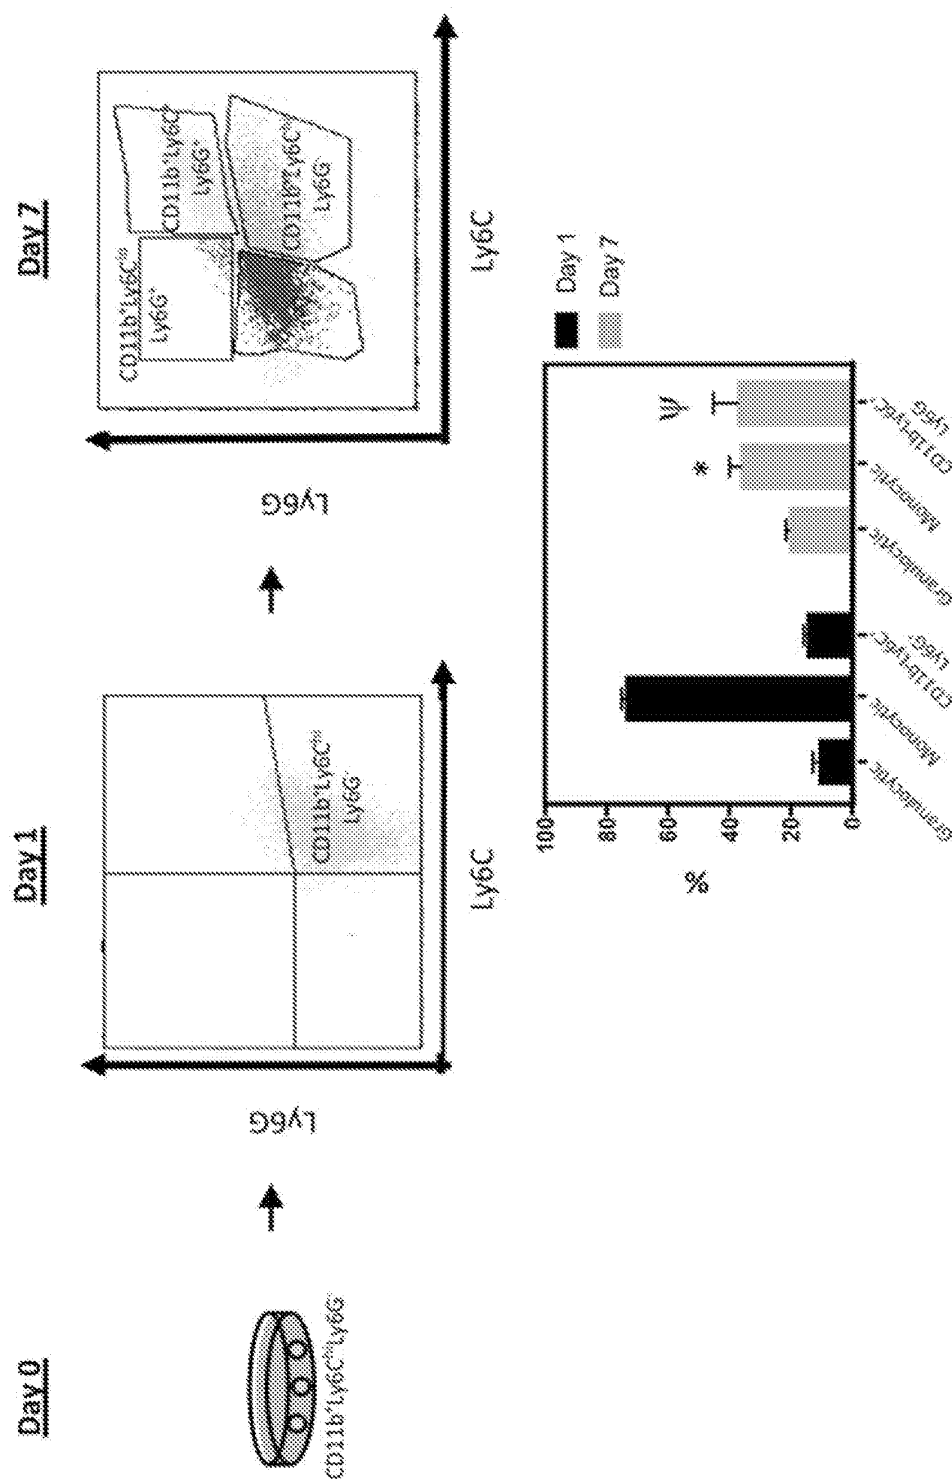


FIG. 12D

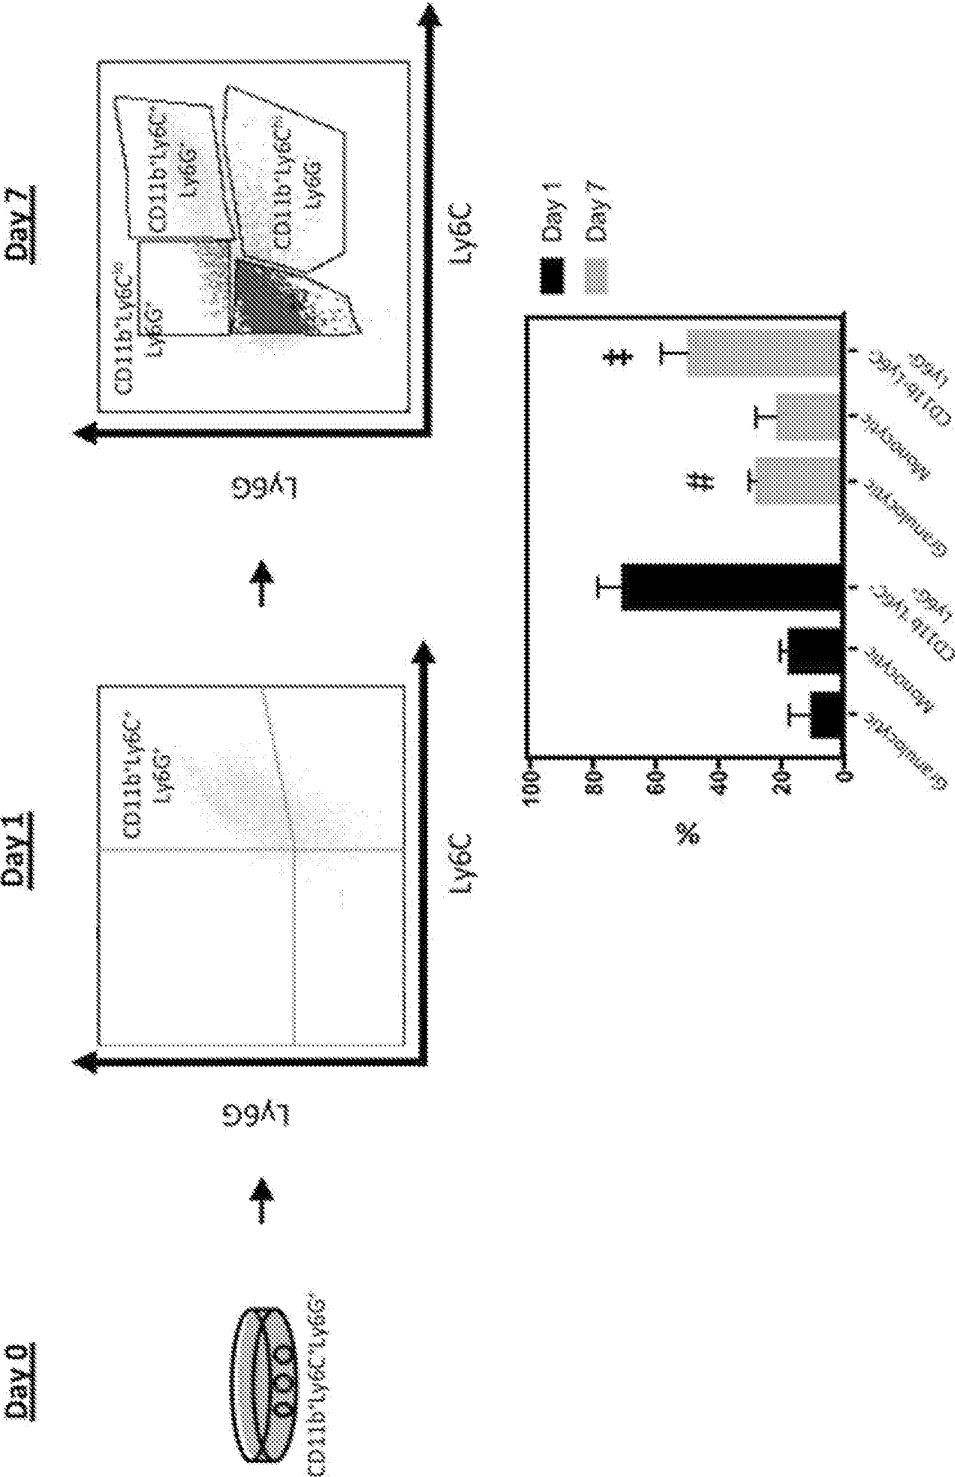


FIG. 12E

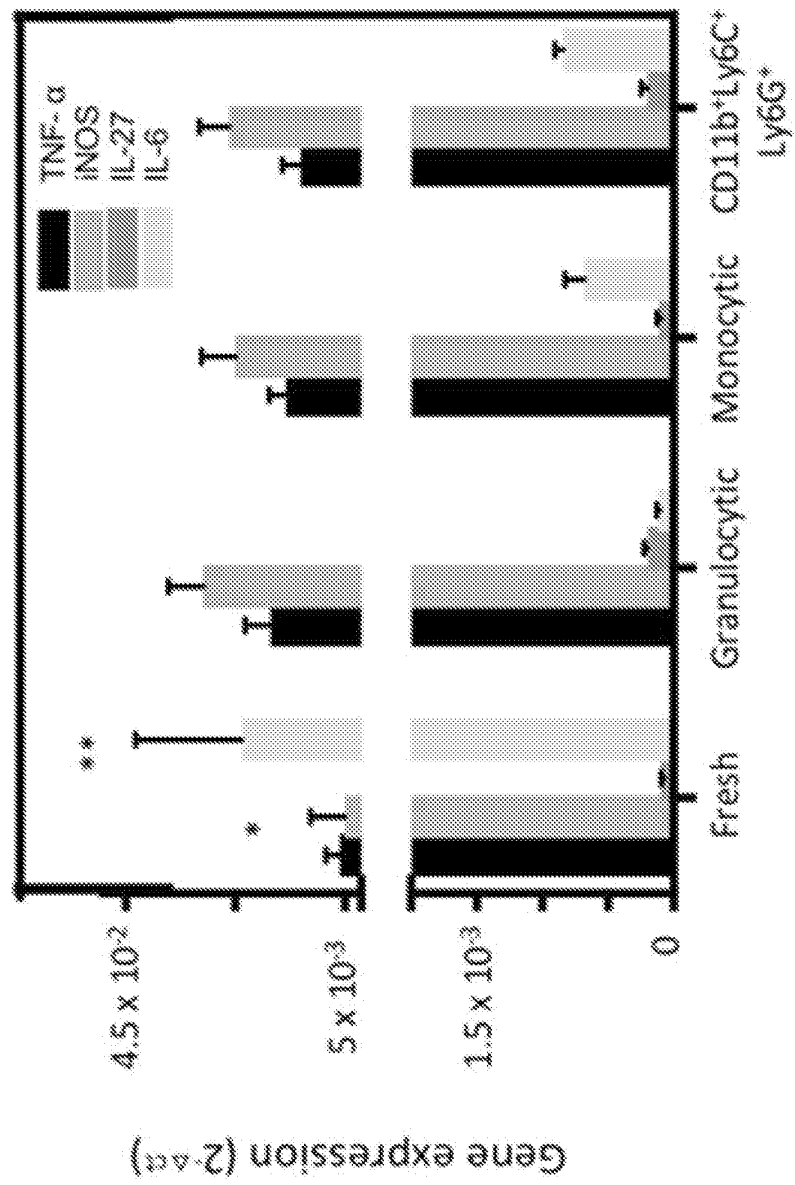


FIG. 12F

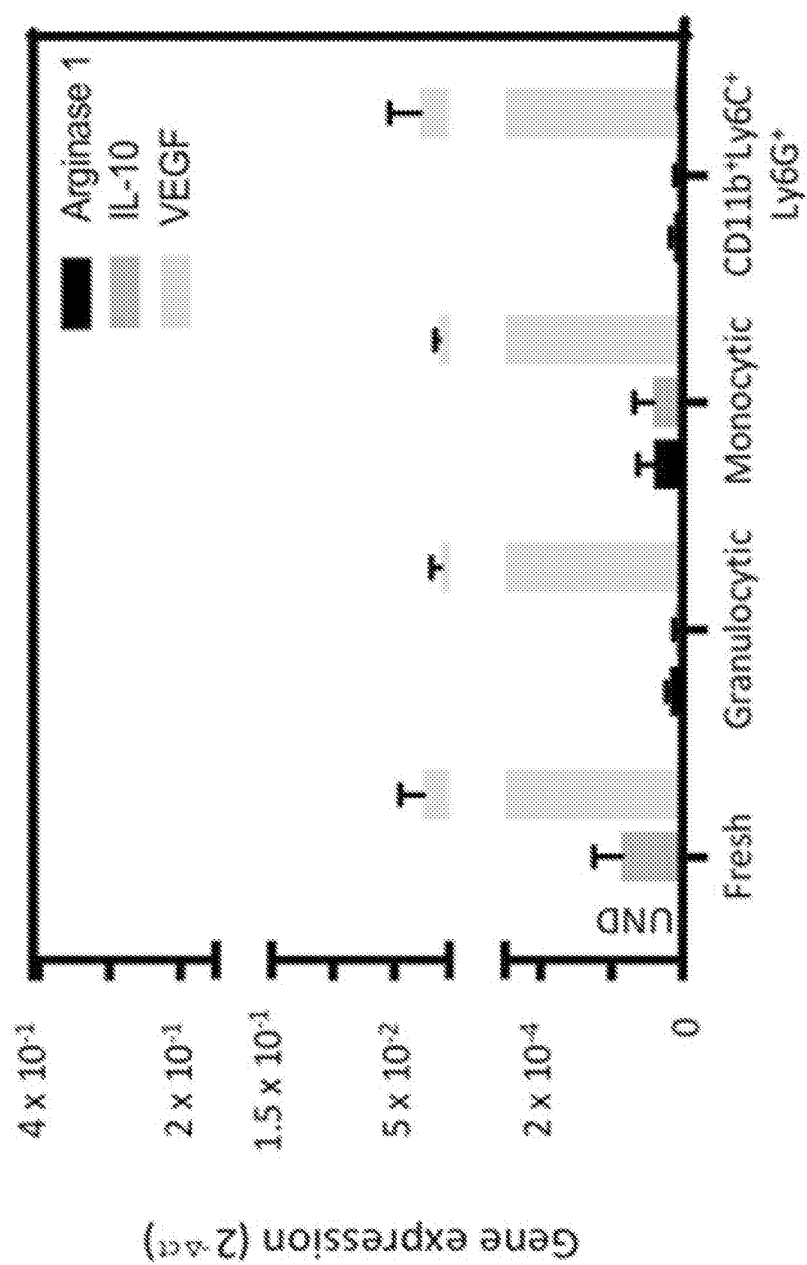


FIG. 12G

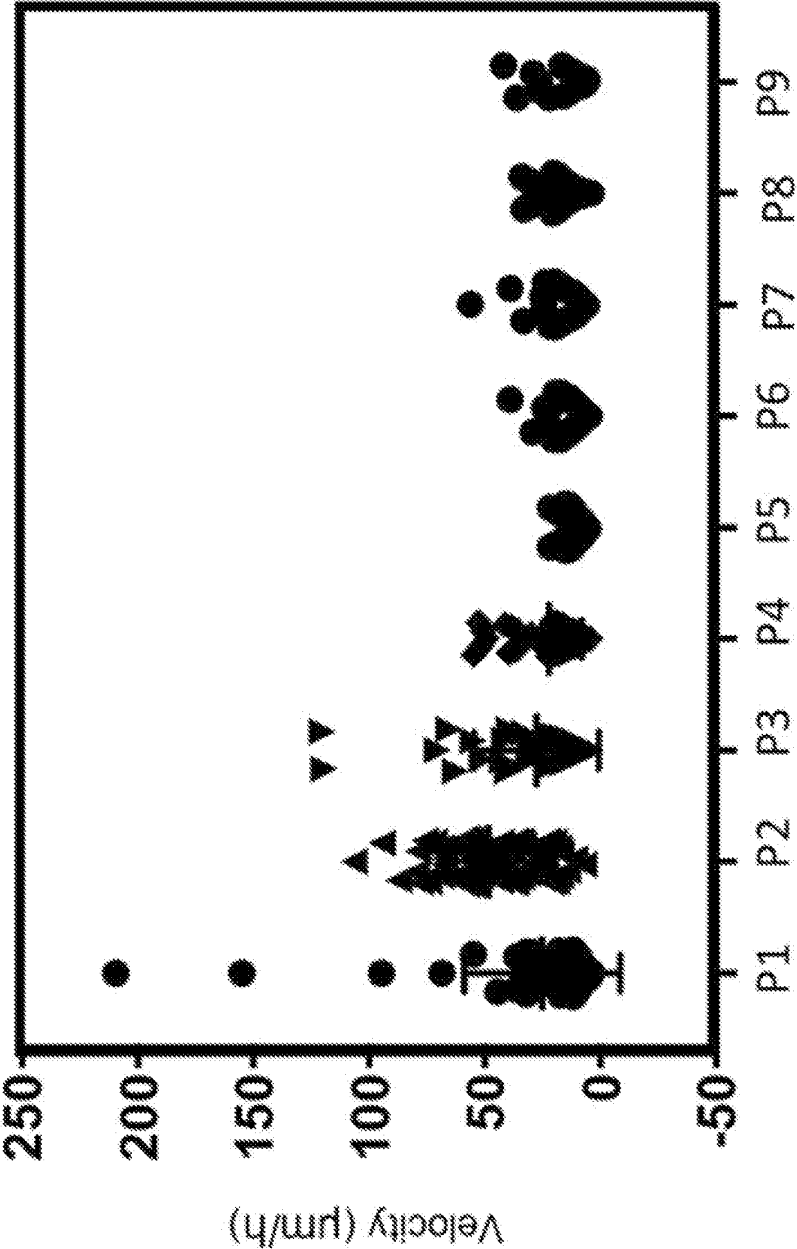


FIG. 13A

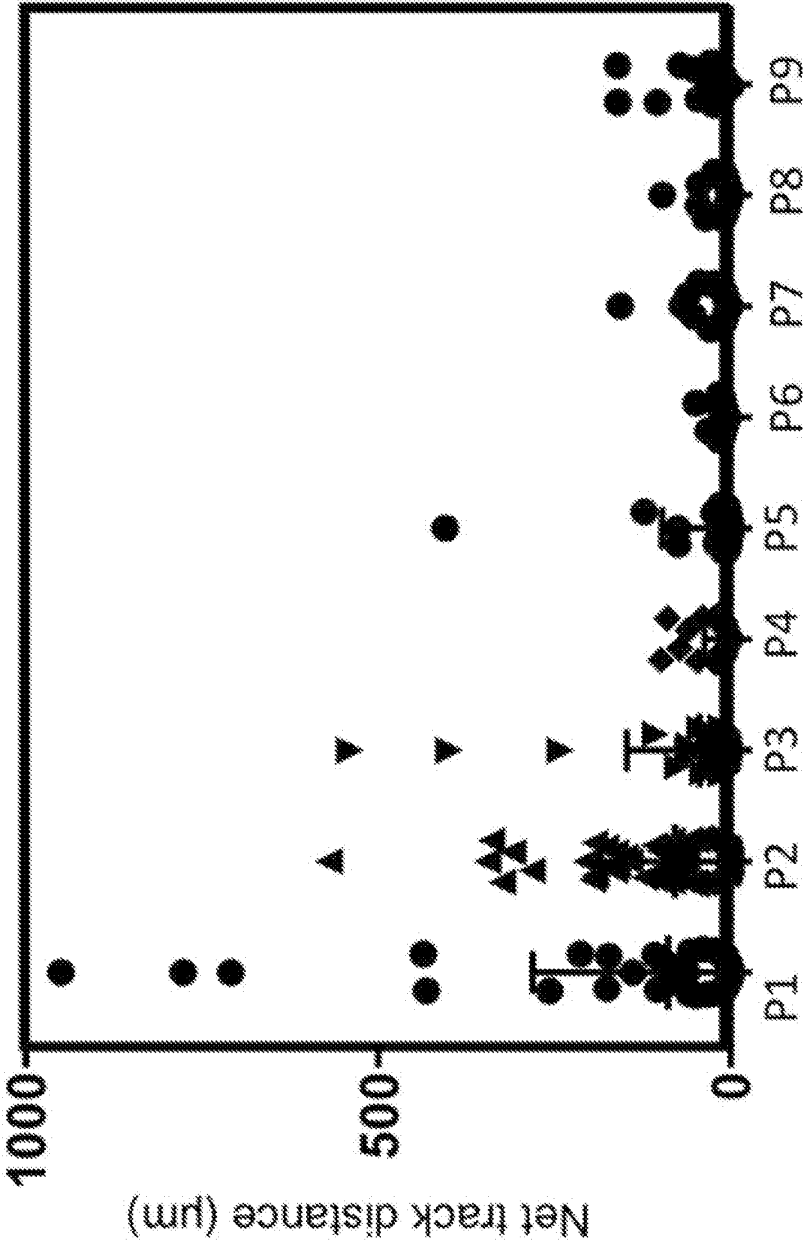


FIG. 13B

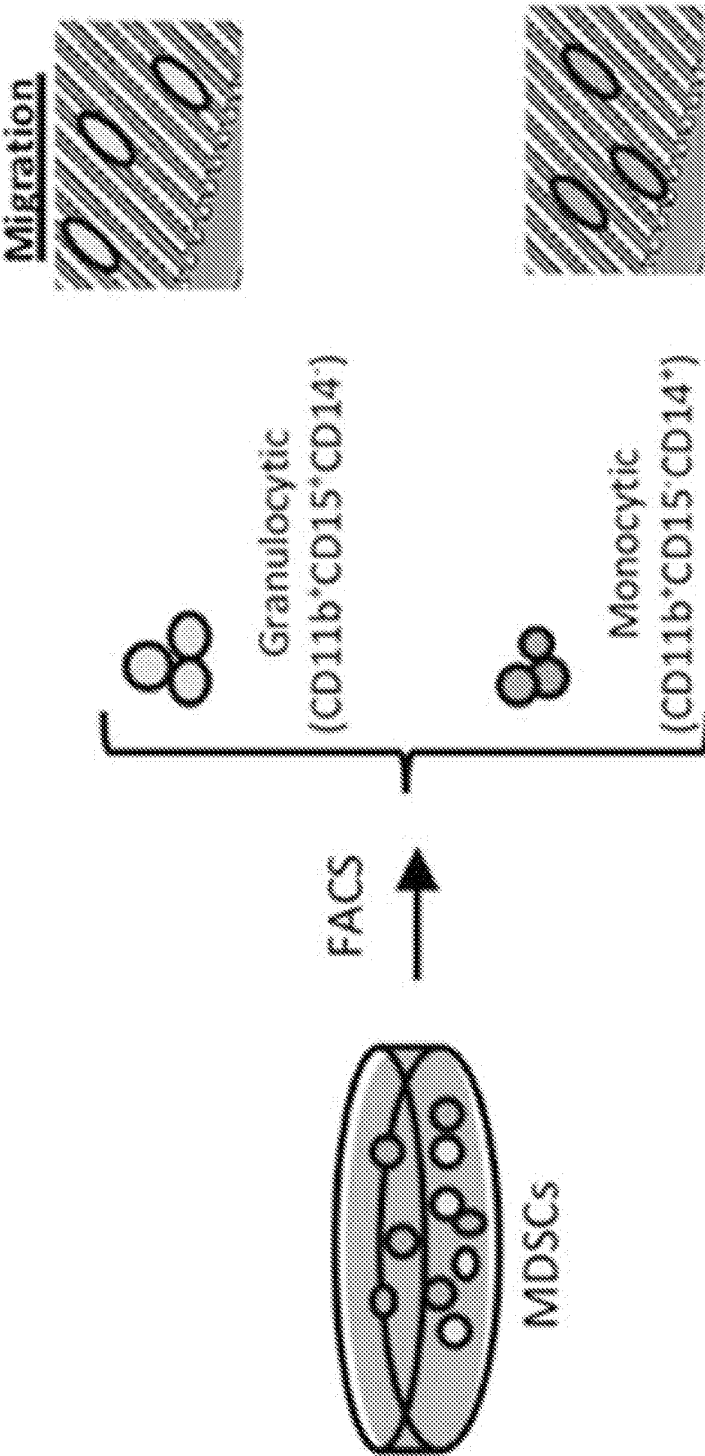


FIG. 14A

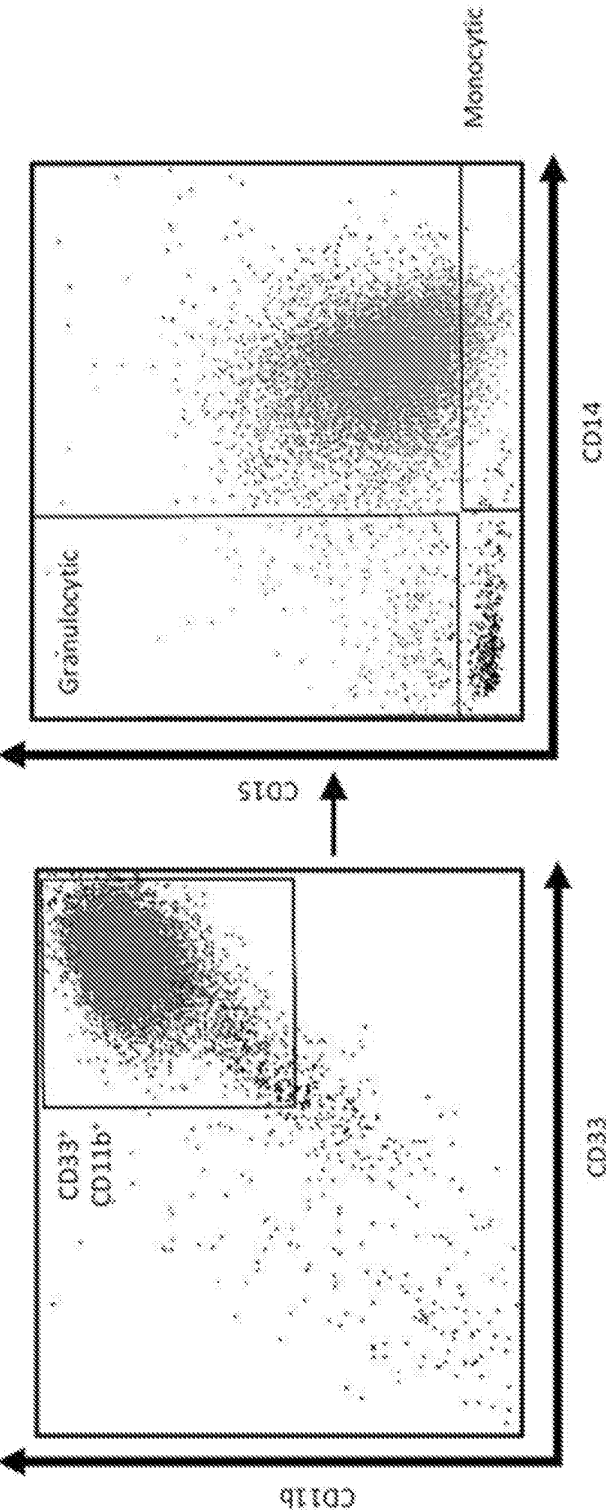


FIG. 14B

FIG. 14C

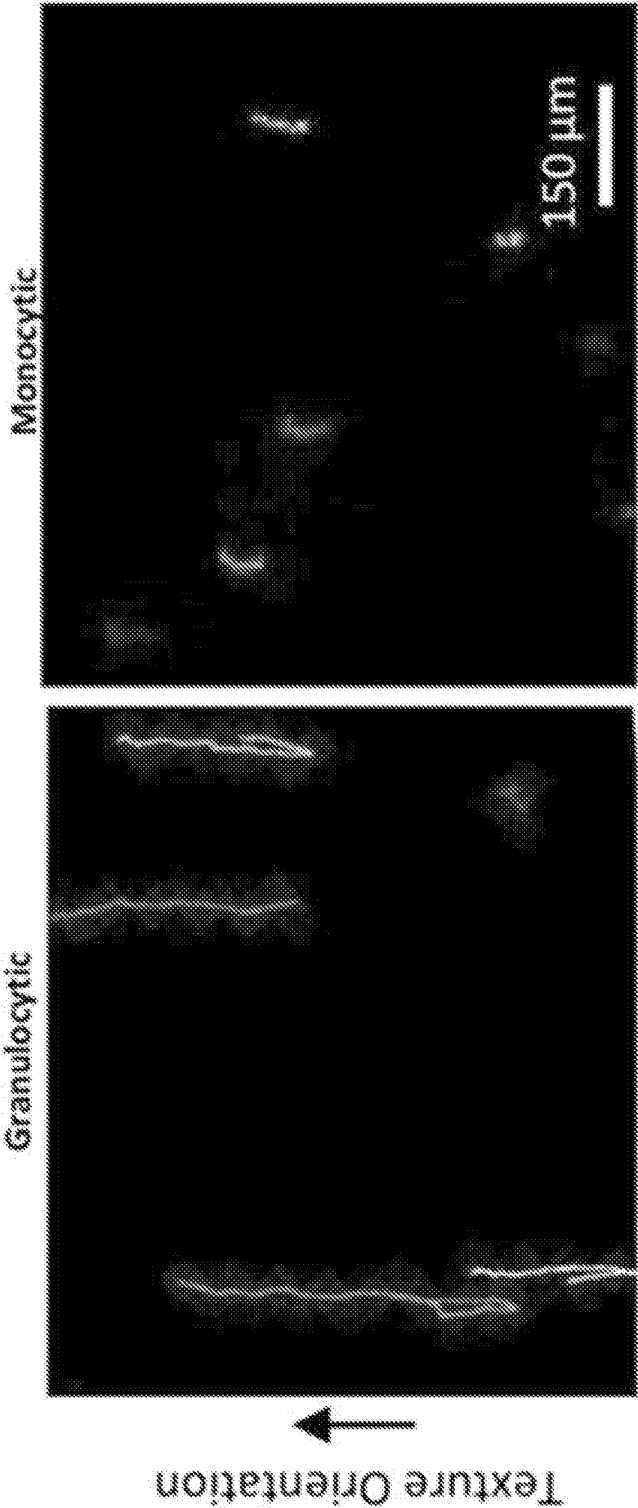


FIG. 14D

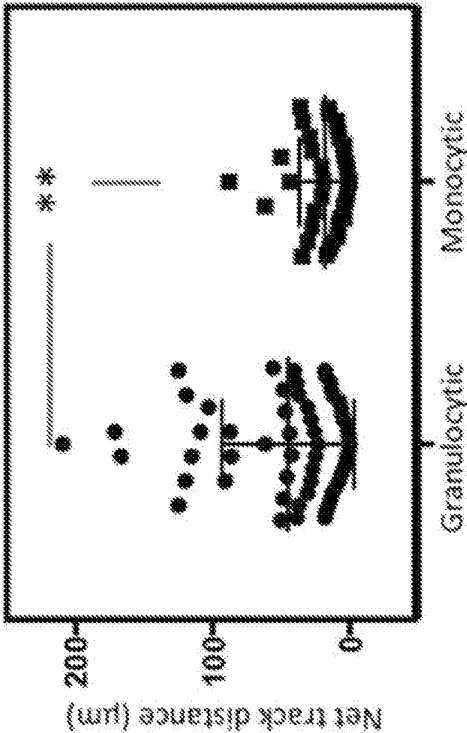


FIG. 14F

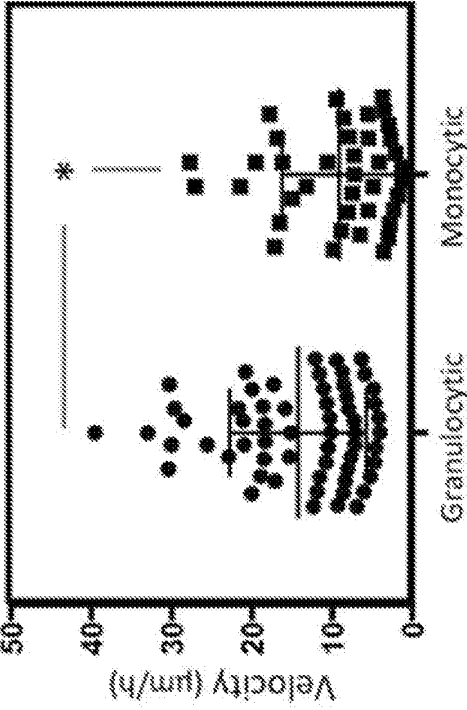


FIG. 14E

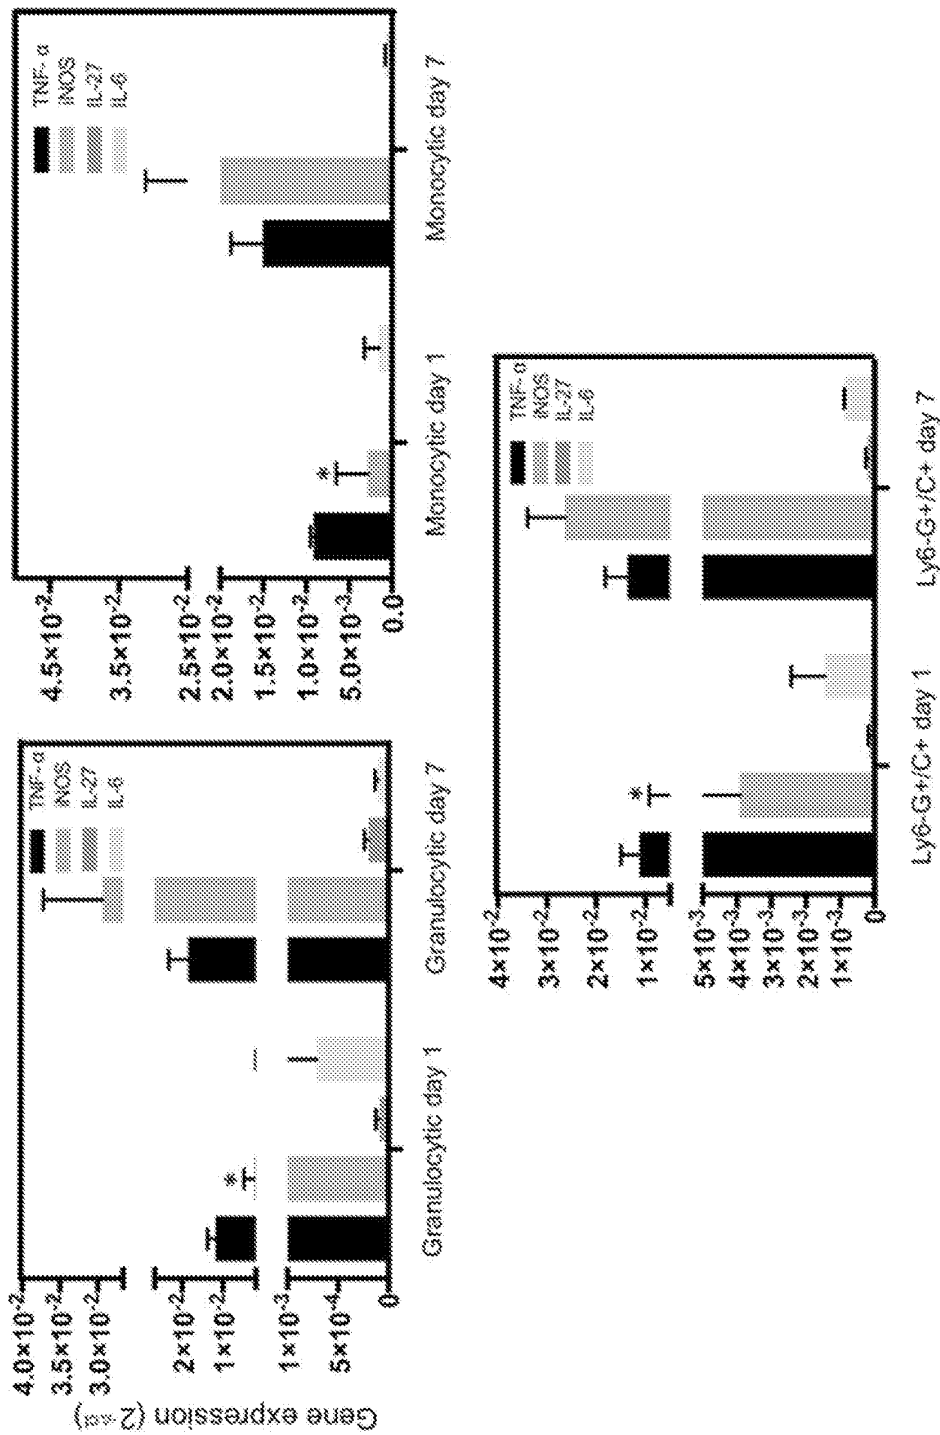


FIG. 15A

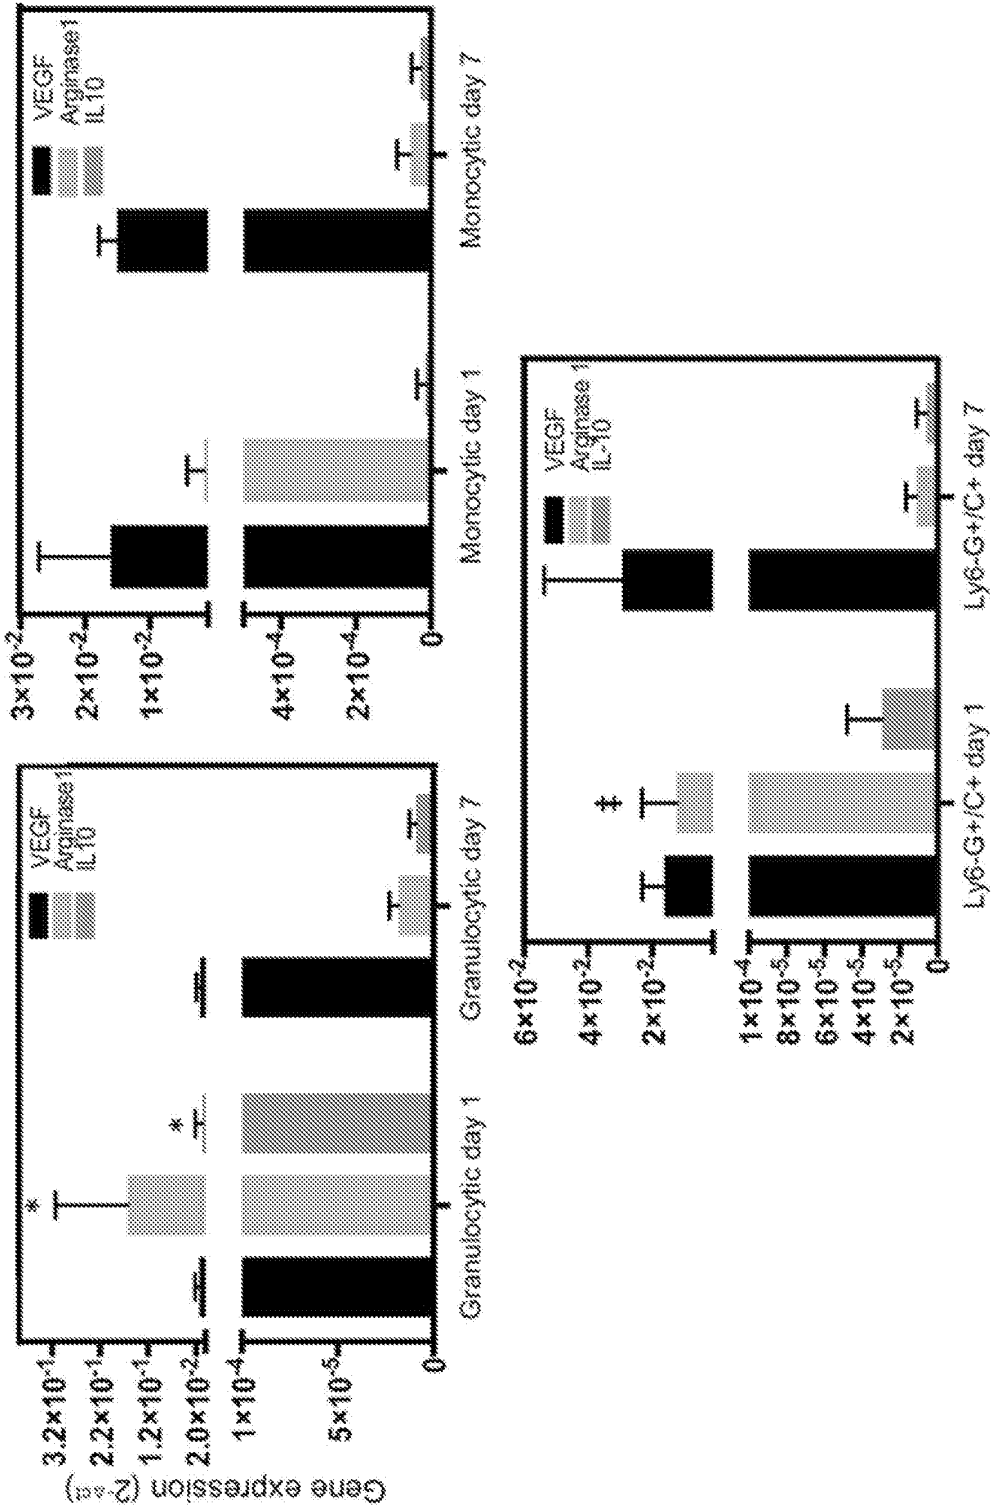


FIG. 15B